



Traceability of Absolute Radiometric Calibration for the Atmospheric Emitted Radiance Interferometer (AERI)

Fred A. Best, Henry E. Revercomb, Robert O. Knuteson, Dave C. Tobin, Ralph G. Dedecker, Tim P. Dirkx, Mark P. Mulligan, Nick N. Ciganovich, Yao Te

**University of Wisconsin
Space Science and Engineering Center**

fred.best@ssec.wisc.edu

**USU/SDL
CALCON 2003**



CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



Abstract

The Atmospheric Emitted Radiance Interferometer (AERI) is a ground-based spectroradiometer that was developed at the University of Wisconsin for the DOE Atmospheric Radiation Measurement (ARM) program to measure the downwelling infrared emission from CO₂, H₂O, and clouds. Twelve continuously operating AERIs are deployed throughout the world, including three marine-based instruments (MAERIs) that are configured to measure sea surface temperature. The AERI instruments are used to improve our understanding of atmospheric radiation transfer and cloud properties for climate studies, and for boundary level temperature and water vapor retrieval and water vapor transport for weather applications.

During operation, the AERI uses two high emissivity blackbody sources to provide instrument absolute calibration accuracies to better than 1% of the ambient radiance. A calibration methodology with traceability to NIST has been successfully implemented for the blackbodies. Absolute radiometric performance of the AERI was verified using the 3rd generation water-bath based NIST blackbody source, with agreement better than 0.065 K over the temperature range from 293 K to 333 K. Instrument repeatability has been demonstrated during a 14 day cruise where two MAERI instruments operating side-by-side measuring sea surface temperature showed agreement to within 0.02 K.

An uncertainty analysis based on the instrument calibration equation was used to allocate the allowable blackbody temperature and emissivity uncertainties. A detailed budget was developed to account for all contributions to both temperature and emissivity uncertainty, including contributions from the instrument spectral calibration. Both temperature and emissivity measurements have traceability to NIST.



Topics

- Overview of AERI and Top Level Radiometric Performance Requirements
- Instrument Calibration Model and Predicted Radiometric Performance
- Blackbody Design and Calibration
- Instrument End-to-end Performance
- Summary



AERI Overview and Radiometric Performance Specification




Slide 4

CALCON 2003
Radiometric Calibration of AERI


THE UNIVERSITY
of
WISCONSIN
MADISON



Atmospheric Emitted Radiance Interferometer (AERI)

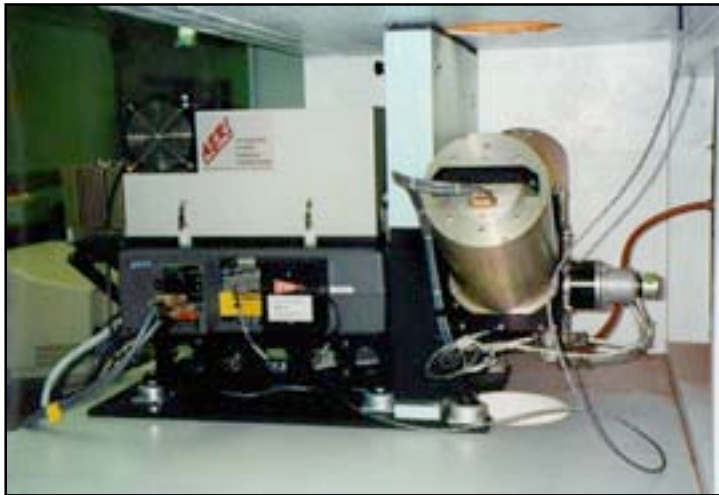

Operational at DOE ARM

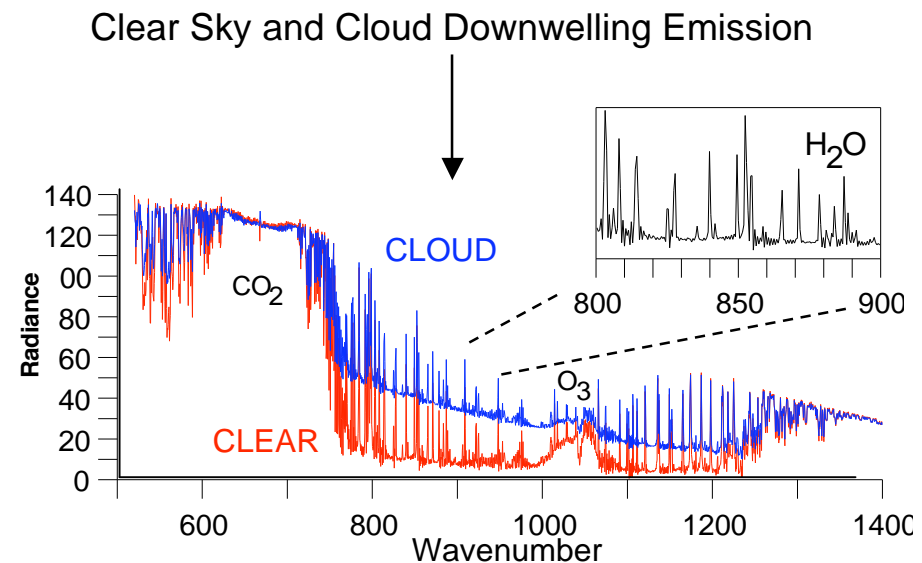


AERI Provides Continuous Accurate High Resolution Radiometry in the Infrared

AERI is used to improve our understanding of atmospheric radiation transfer and cloud properties for climate studies, and for weather applications.



AERI Provides Continuous Atmospheric Profiling of Temperature and Water Vapor

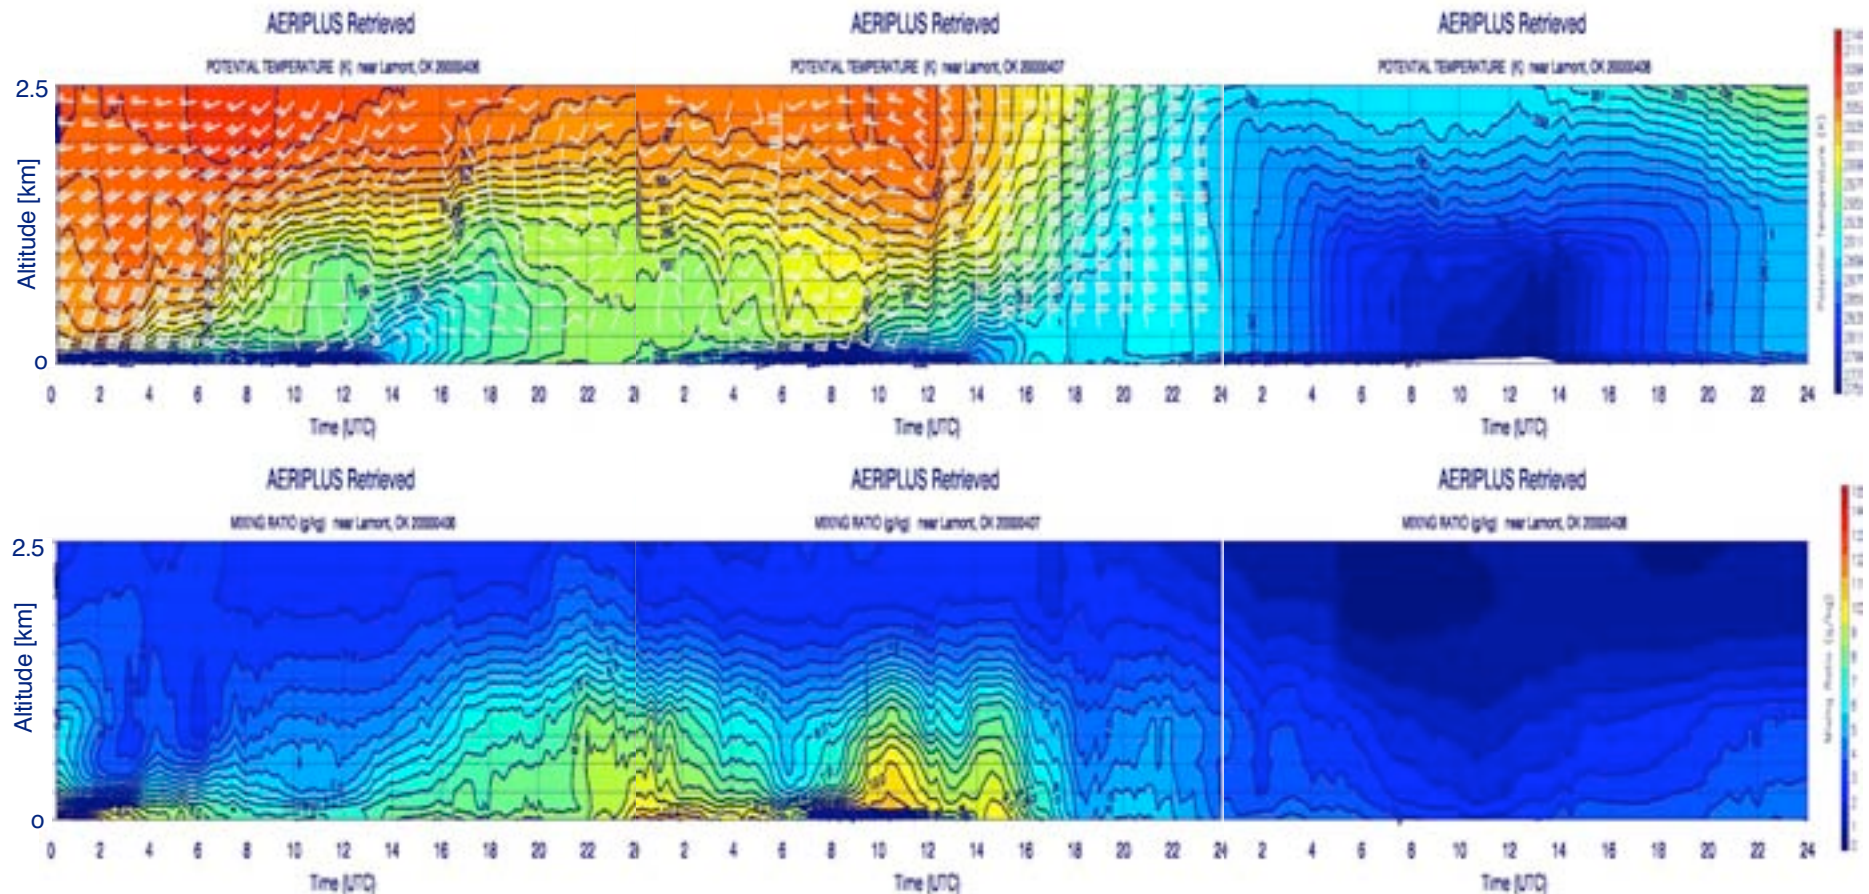



Slide 6

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



AERI Systems Around The World

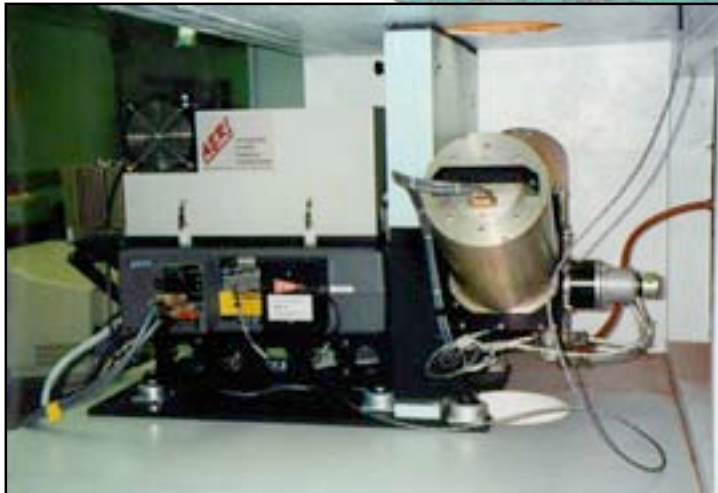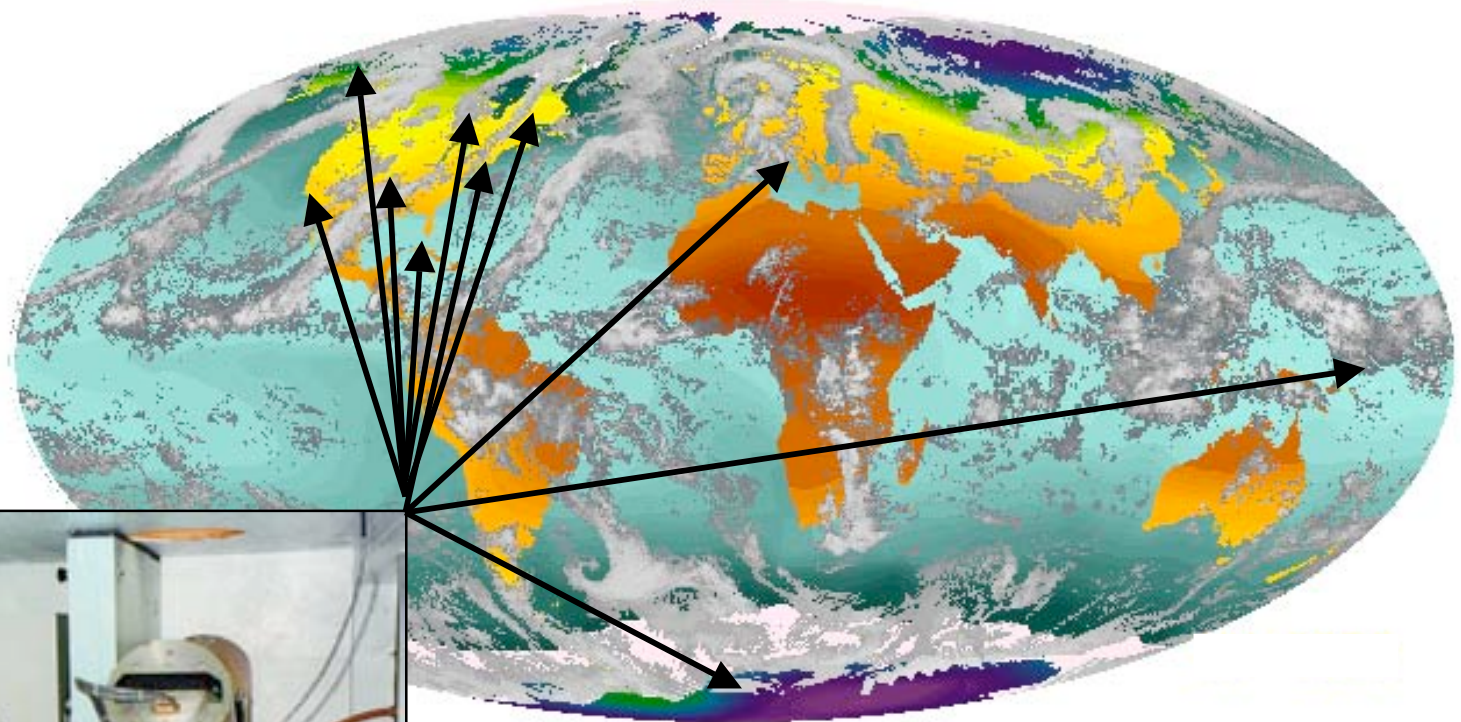

- UW AERI - 2 (AERIBAGO, SSEC)
- DOE AERI - 7 (Kansas/Oklahoma, Alaska, S. Pacific)
- U-Miami M-AERI - 3 (Florida)
- Bomem AERI - 4 (Italy, California, Maryland, Canada)
- U Idaho P-AERI - 1 (Antarctica)




Slide 7

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



AERI Interferometer Assembly

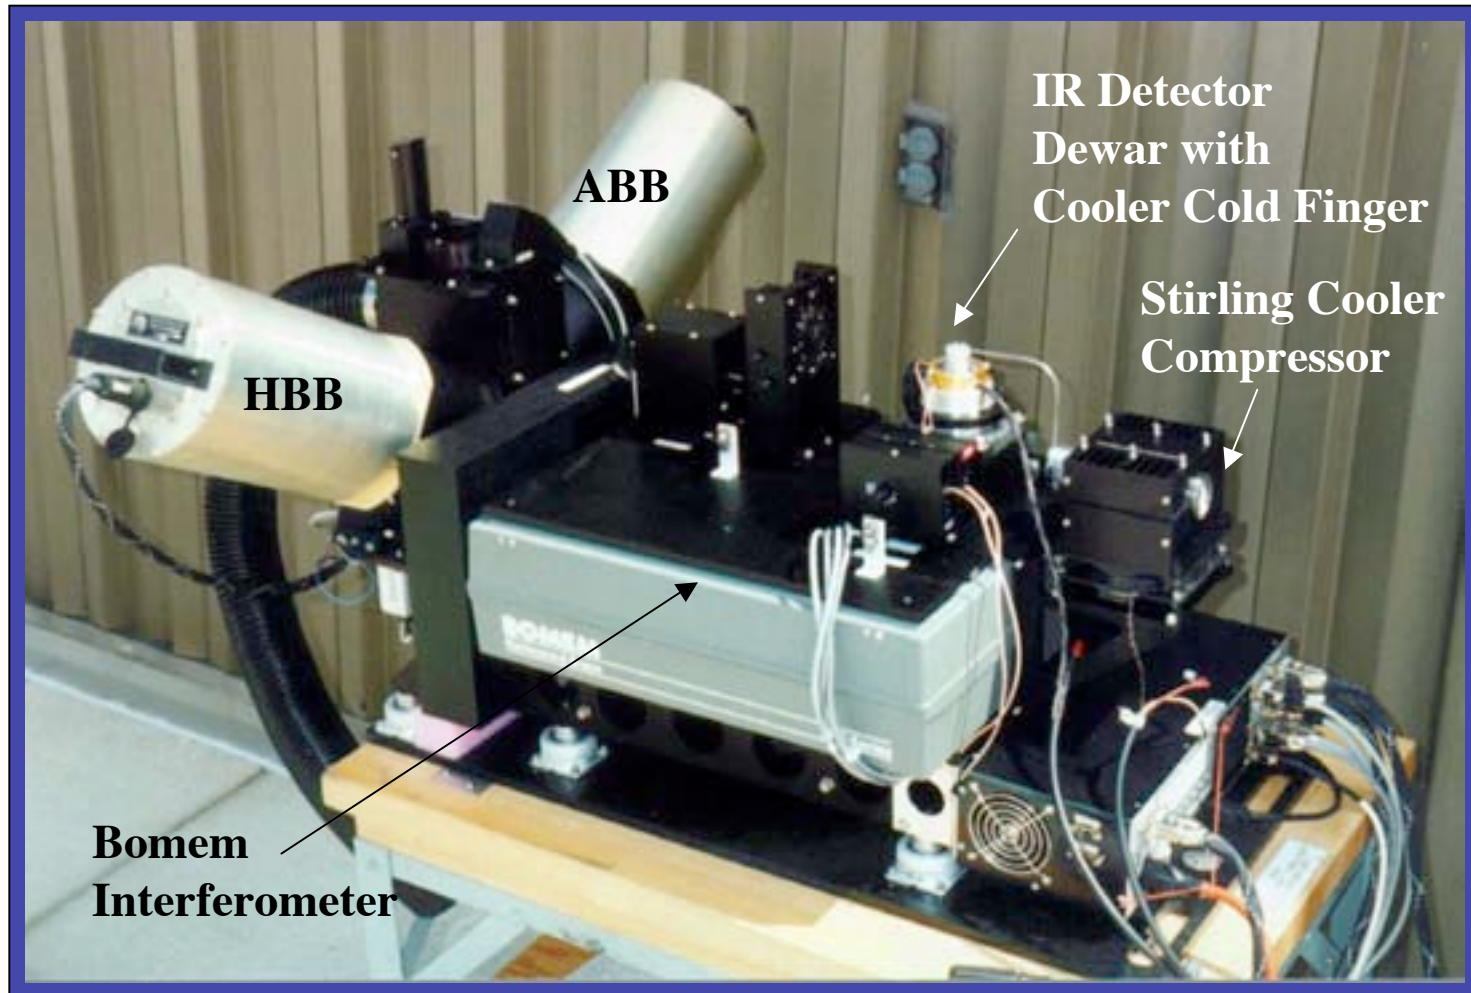

Slide 8

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



AERI Front-end Assembly





Interferometer Assembly with Blackbodies



Detector with Stirling Cooler

**Front-end Port
for Scene Mirror
Assembly**

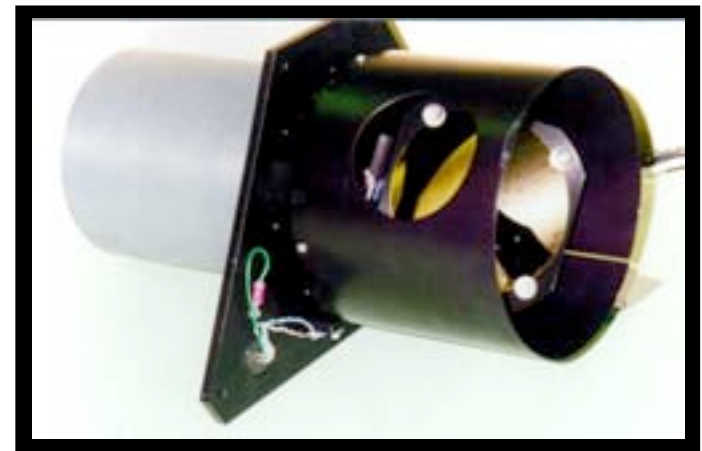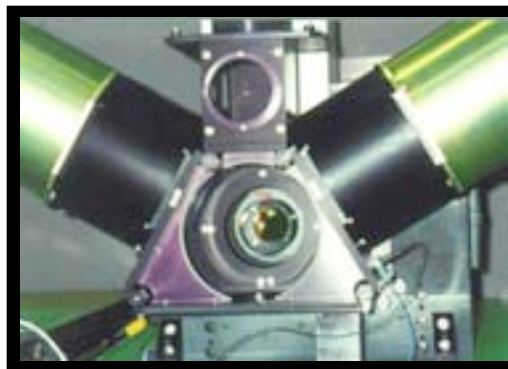


Scene Mirror Assembly



AERI Functional Block Diagram

Interferometer Assembly

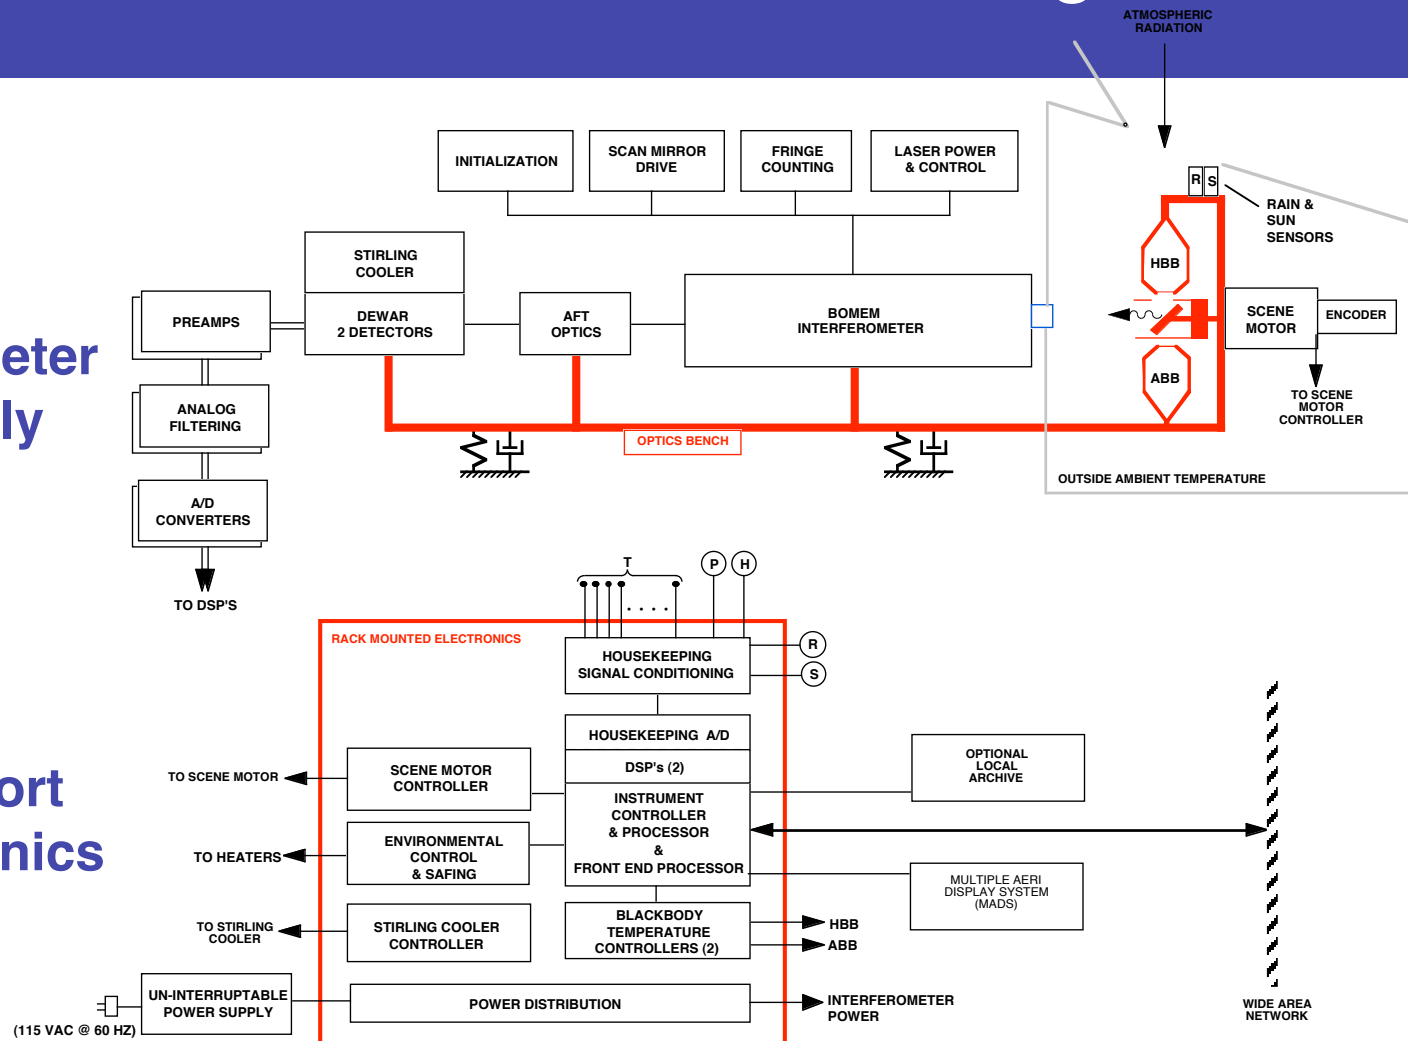

AERI Radiometric Accuracy Requirements

- Absolute Accuracy: better than 1%*
- Reproducibility: better than 0.2%*

*expressed as % of ambient radiance



Radiance Uncertainty Requirements and Budget

❑ Top Level Requirements

- Absolute Accuracy: **< 1.0% of ambient radiance**
- Reproducibility: **< 0.2% of ambient radiance**

❑ Budget Goals for Key Contributors


	Absolute	Reprod.
Detector Non-linearity Correction <i>(addressed briefly here)</i>	0.2%	0.05%
Blackbody Calibration <i>(main topic of this talk)</i>	0.9%	0.18%
Spectral Calibration <i>(material in Dave Tobin's talk applies)</i>	0.2%	0.05%
	0.95%	0.20%

All numbers are 3 σ (“not to exceed”)




AERI Non-linearity Correction and Uncertainty

Sky view and ABB radiance spectra

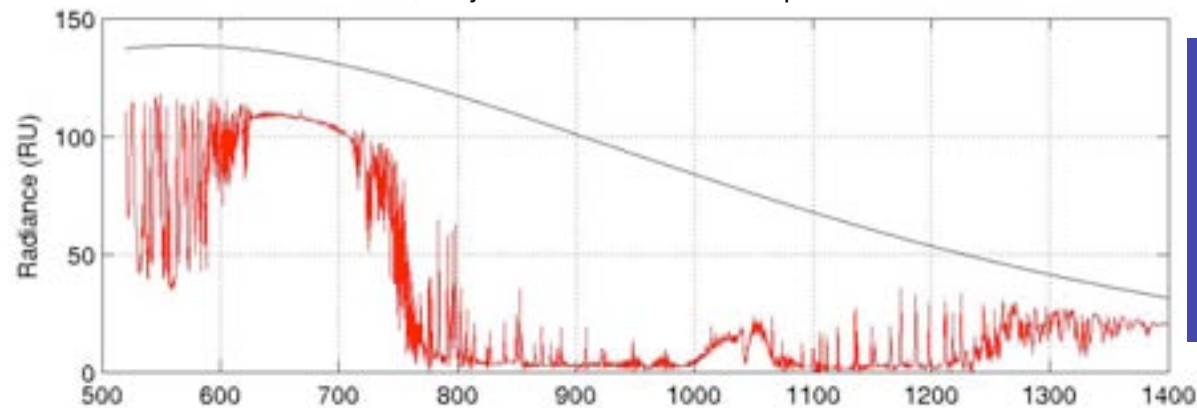

**Maximum Detector
Non-linearity
correction is order
1%**

uncertainty in nonlinearity correction

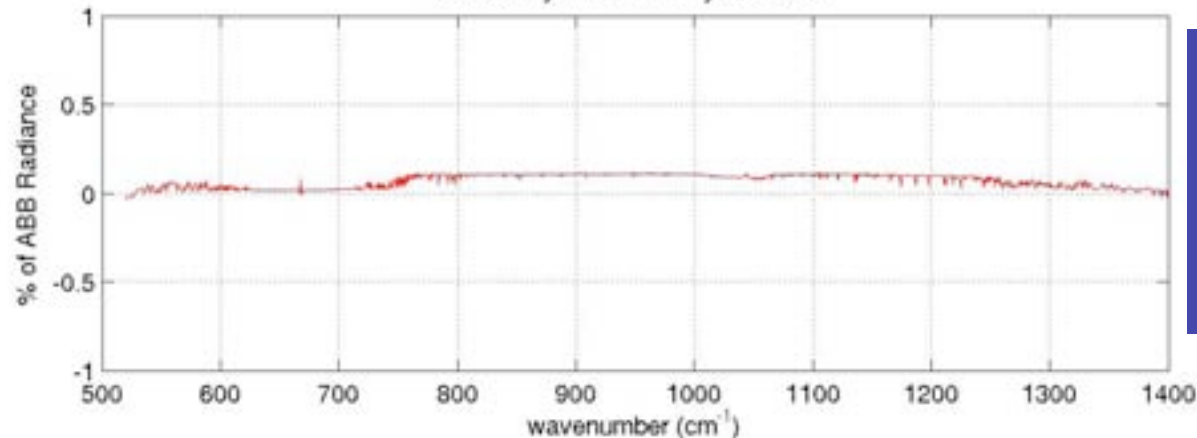

**Uncertainty in
correction is
estimated to be
< 0.10%**

The non-linearity correction is physically based with one adjustable and one modeled parameter



Instrument Calibration Model and Predicted Radiometric Performance



Slide 14

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



AERI Instrument Calibration Equation


$$N = (B_H - B_A) \operatorname{Re} \left[\frac{C_S - C_A}{C_H - C_A} \right] + B_A$$

- N is the calibrated spectral radiance
- B_H is the effective Planck emission for the hot blackbody
- B_A is the effective Planck emission for the ambient blackbody
- C_S is the complex spectrum for the sky view
- C_H is the complex spectrum for the hot blackbody view
- C_A is the complex spectrum for the ambient blackbody view
- $\operatorname{Re}()$ is the real part of the complex ratio




AERI Calibration Error Estimates

Radiometric Requirement is 0.9% of Ambient Radiance

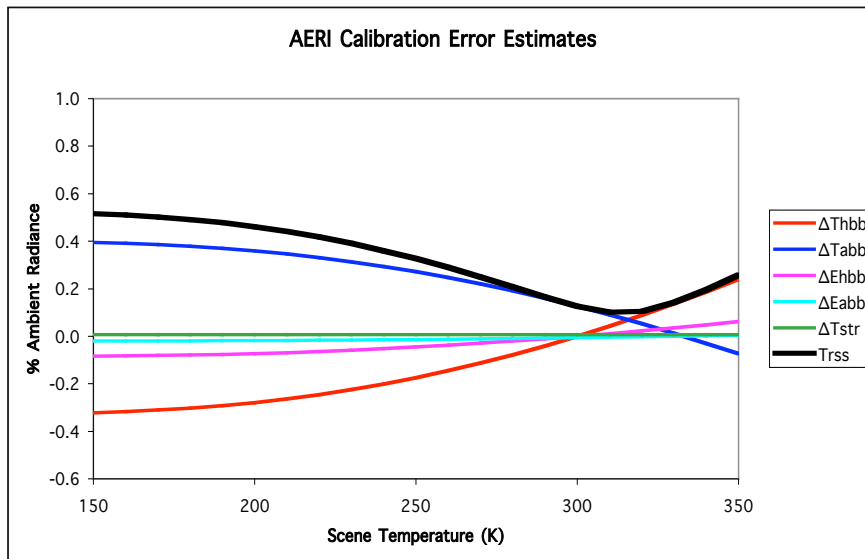

Input Parameters		Uncertainties (3 sigma)	
wn	770	Wavenumber, [cm-1]	
Thbb	333	Temp. of Hot Blackbody, [K]	$\Delta Thbb$ 0.10 [K]
Tcbb	300	Temp. of Cold Blackbody, [K]	$\Delta Tcbb$ 0.10 [K]
Tstr	305	Temp. of Structure Reflecting into BB's, [K]	$\Delta Tstr$ 5 [K]
Ehbb	0.999	Emissivity of HBB, [-]	$\Delta Ehbb$ 0.001 [-]
Ecbb	0.999	Emissivity of CBB, [-]	$\Delta Ecbb$ 0.001 [-]

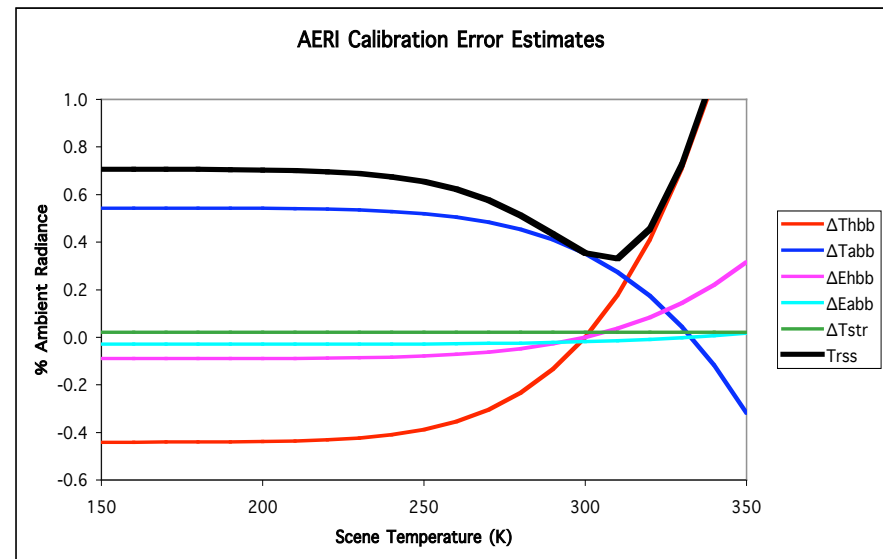

Input Parameters		Uncertainties (3 sigma)	
wn	2200	Wavenumber, [cm-1]	
Thbb	333	Temp. of Hot Blackbody, [K]	$\Delta Thbb$ 0.10 [K]
Tcbb	300	Temp. of Cold Blackbody, [K]	$\Delta Tcbb$ 0.10 [K]
Tstr	305	Temp. of Structure Reflecting into BB's, [K]	$\Delta Tstr$ 5 [K]
Ehbb	0.999	Emissivity of HBB, [-]	$\Delta Ehbb$ 0.001 [-]
Ecbb	0.999	Emissivity of CBB, [-]	$\Delta Ecbb$ 0.001 [-]


Longwave: 770 cm-1

Shortwave: 2200 cm-1




AERI Reproducibility Error Estimates

Radiometric Requirement is 0.18% of Ambient Radiance

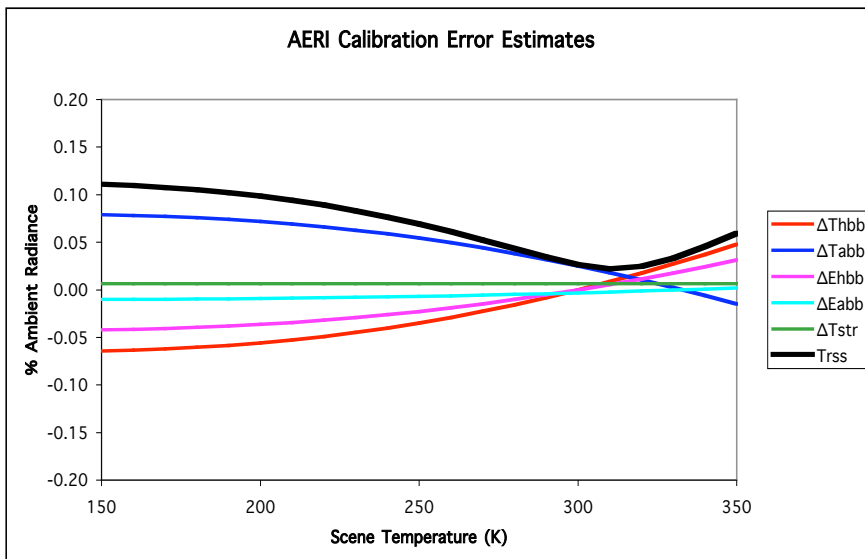

Input Parameters		Uncertainties (3 sigma)	
wn	770	Wavenumber, [cm-1]	
Thbb	333	Temp. of Hot Blackbody, [K]	$\Delta Thbb$ 0.02 [K]
Tcbb	300	Temp. of Cold Blackbody, [K]	$\Delta Tcbb$ 0.02 [K]
Tstr	305	Temp. of Structure Reflecting into BB's, [K]	$\Delta Tstr$ 5 [K]
Ehbb	0.999	Emissivity of HBB, [-]	$\Delta Ehbb$ 0.0005 [-]
Ecbb	0.999	Emissivity of CBB, [-]	$\Delta Ecbb$ 0.0005 [-]

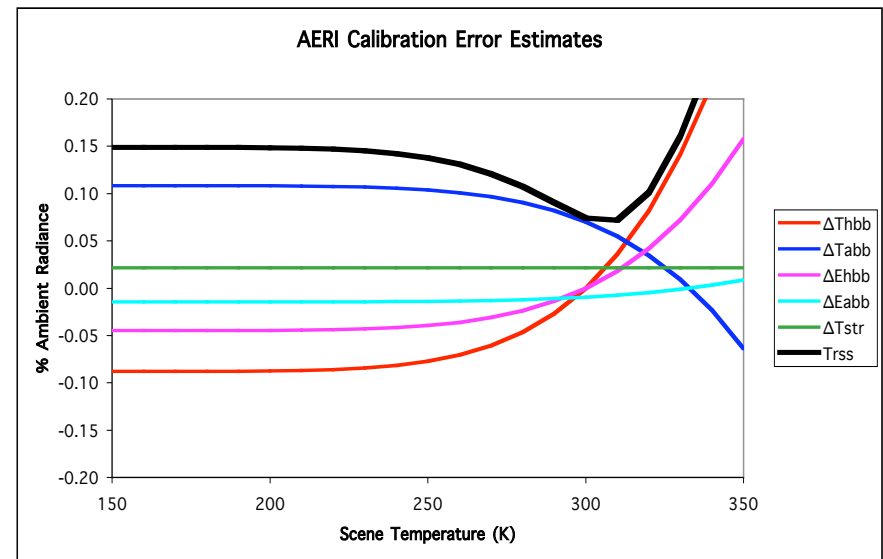

Input Parameters		Uncertainties (3 sigma)	
wn	2200	Wavenumber, [cm-1]	
Thbb	333	Temp. of Hot Blackbody, [K]	$\Delta Thbb$ 0.02 [K]
Tcbb	300	Temp. of Cold Blackbody, [K]	$\Delta Tcbb$ 0.02 [K]
Tstr	305	Temp. of Structure Reflecting into BB's, [K]	$\Delta Tstr$ 5 [K]
Ehbb	0.999	Emissivity of HBB, [-]	$\Delta Ehbb$ 0.0005 [-]
Ecbb	0.999	Emissivity of CBB, [-]	$\Delta Ecbb$ 0.0005 [-]

Longwave: 770 cm-1

Shortwave: 2200 cm-1



Blackbody Design and Calibration



Slide 18

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



Blackbody Requirements

❑ Blackbody System Requirements

- Temperature knowledge: ± 0.10 K
- Temp. gradient knowledge: better than 0.10 K
- Emissivity: > 0.998
- Emissivity knowledge: better than $\pm 0.1\%$

❑ Instrument Imposed Requirements

- BB Aperture: 6.9 cm
- Envelope: 18 cm dia. X 30 cm long
- Operating Temperature: 213 K to 333 K
- Period between cal. views: < 10 minutes



Top-level Design Choices

❑ **Cavity Approach**

- Provides high emissivity (cavity factor near 40)
- Emissivity enhancement due to cavity is well characterized
- Cavity walls provide good conduction (low gradients)
- Easy to manufacture

❑ **Chemglaze Z306 Black Paint**


- Provides high emissivity that is well characterized and stable
- Provides a hardy diffuse surface

❑ **YSI 46041 Super-stable Thermistors**



- Very stable ($< 0.01^{\circ}\text{C}$ drift after 100 months at 70°C)
- Easy to couple thermally to blackbody cavity
- Reasonably rugged



AERI Blackbody

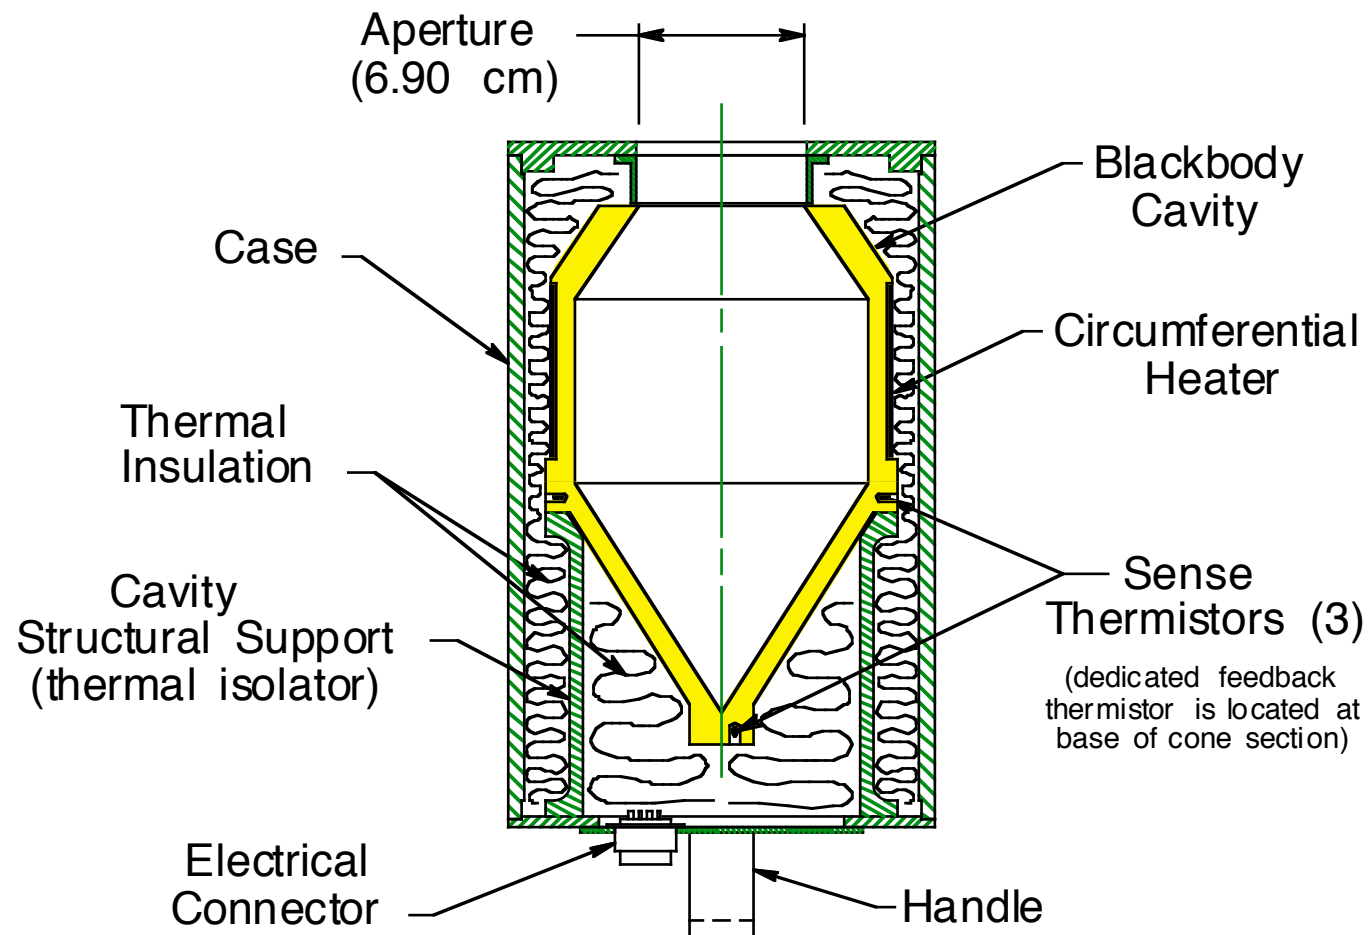


AERI Blackbody

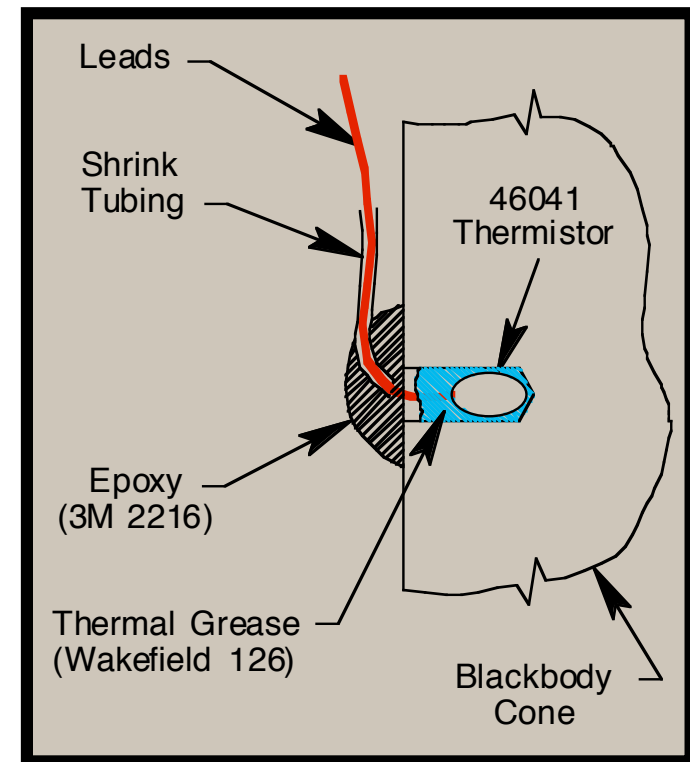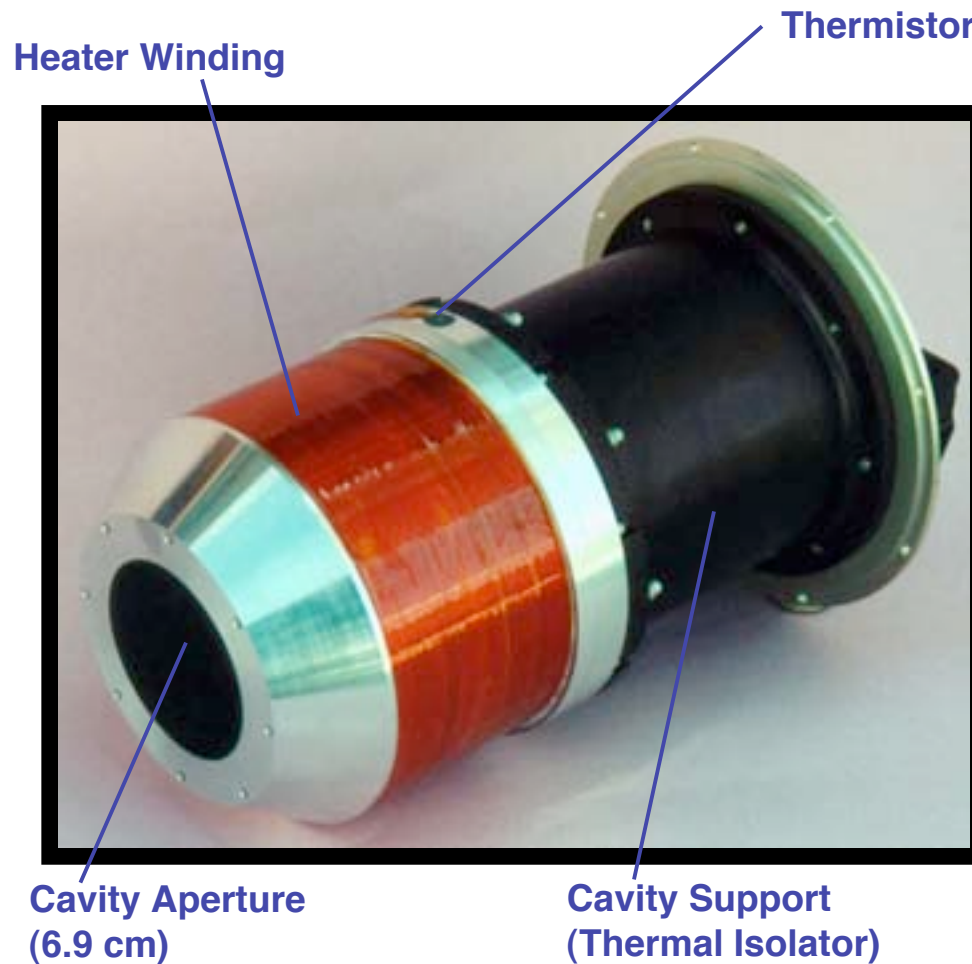

Thermistor Installation




AERI Blackbody Calibration Roadmap

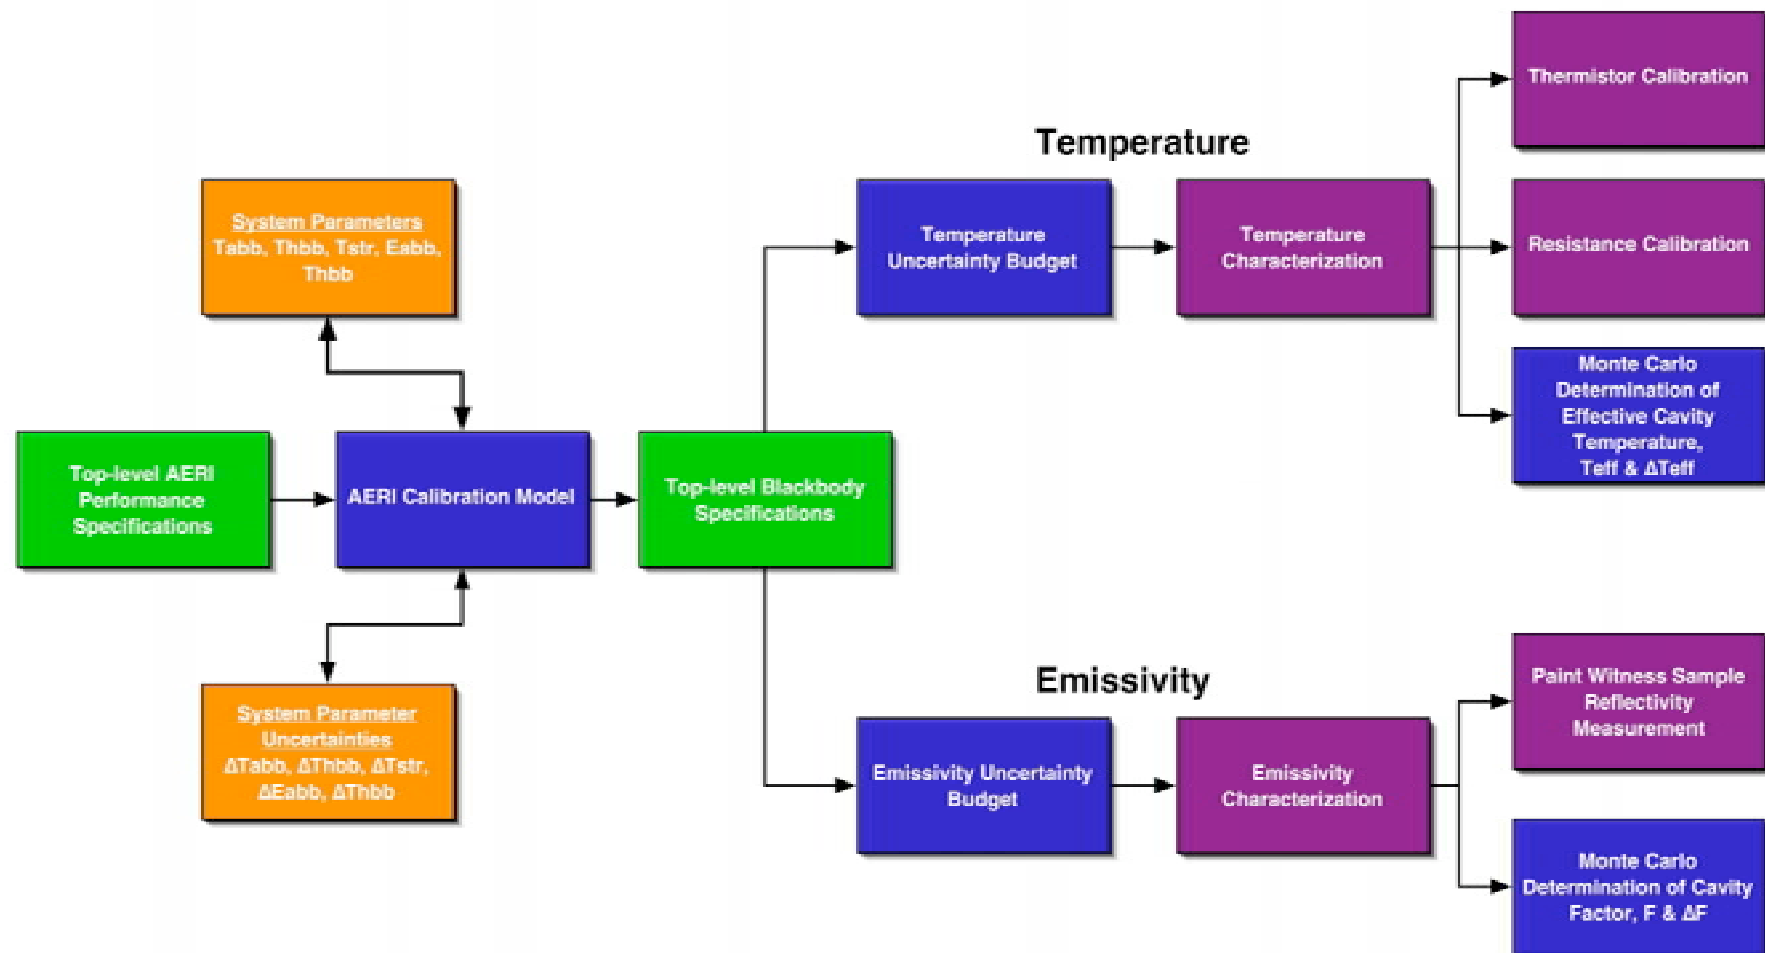


AERI Blackbody Temperature Calibration Overview


AERI BB System

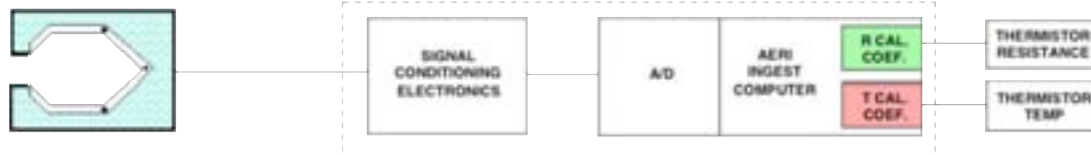

Resistance Calibration

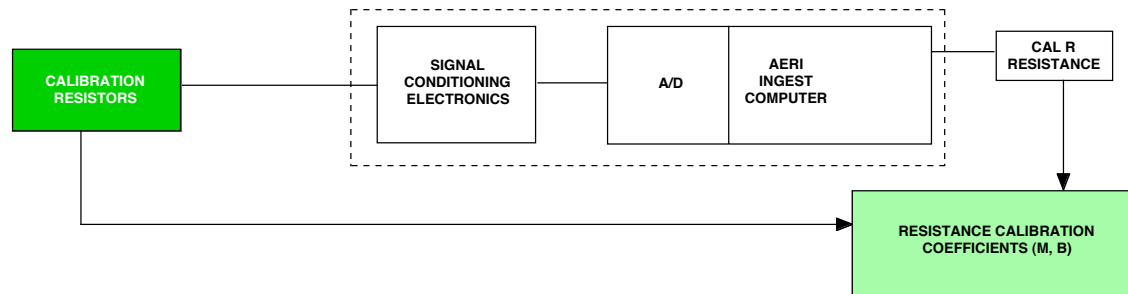

Temperature Calibration

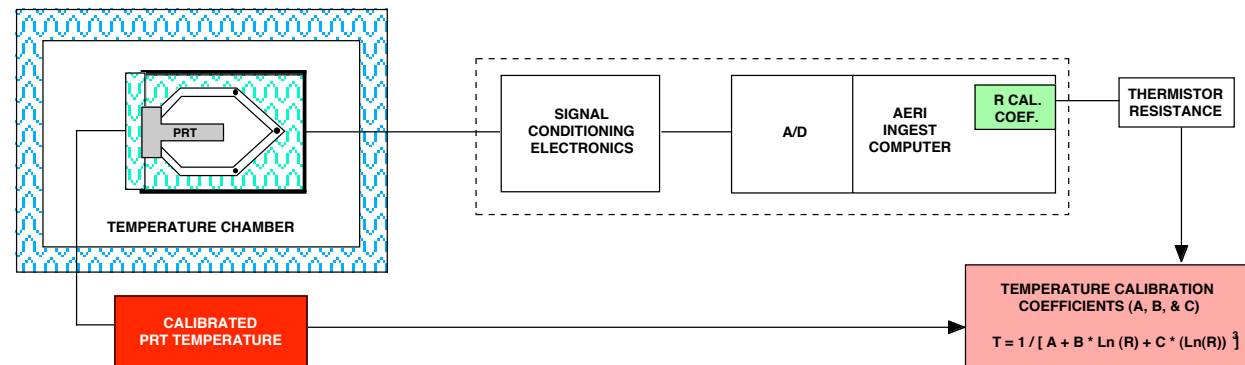


Temperature Uncertainty Budget

Temperature and Resistance Reference Uncertainty		\pm peak error [K]	RSS [K]
26	Temperature Calibration Standard (Guildline PRT)	0.030	0.032
32	Calibration Resistors	0.007	
33	Resistor Readout Electronics Residual Error	0.007	
RSS		0.032	
Thermistor Temperature Transfer Uncertainty			
26	Temperature Gradient Between PRT and Thermistors	0.020	0.020
28	Calibration Fitting Equation Residual Error	0.003	
RSS		0.020	
Cavity Temperature Non-uniformity Uncertainty			
37	Azumuthal Gradients Due to Free Convection		0.058
37	Longitudinal Gradients Due Primarily to Conduction		
37	Radial Gradients Due to Conduction, Convection, and Radiation		
29	Paint Gradient		
RSS		0.058	
Long-term Stability			
30	Thermistor	0.050	0.058
34	Resistance Measurement Electronics	0.030	
RSS		0.058	
Effective Radiometric Temperature Weighting Factor Uncertainty			
36	Monte Carlo Ray Trace Model Uncertainty in Determining Teff	0.030	0.030
			0.095
XX	Indicates slide number where more detailed information is presented		



AERI Blackbody Temperature Calibration- Probe Traceability & Configuration

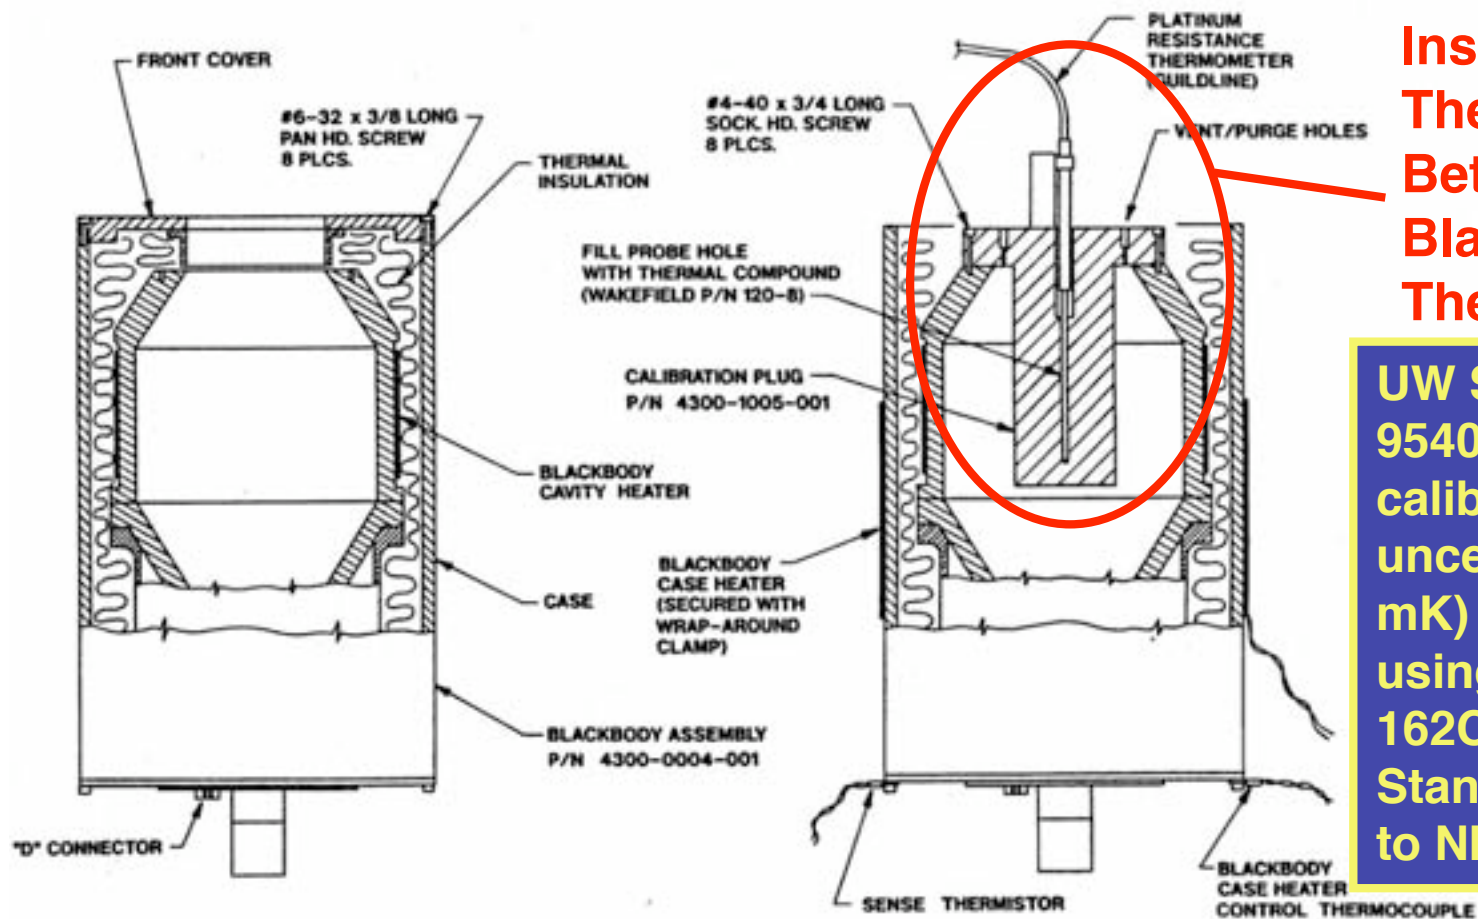

Insures Excellent Thermal Coupling Between PRT and Blackbody Thermistors


UW SSEC Guildline 9540 PRT is calibrated (with an uncertainty of 30 mK) at the factory using a Rosemont 162CE SPRT Primary Standard Traceable to NIST.

Standard Configuration

Calibration Configuration




AERI Thermistor Calibrations Reduce Uncertainty From YSI Nominal Specification

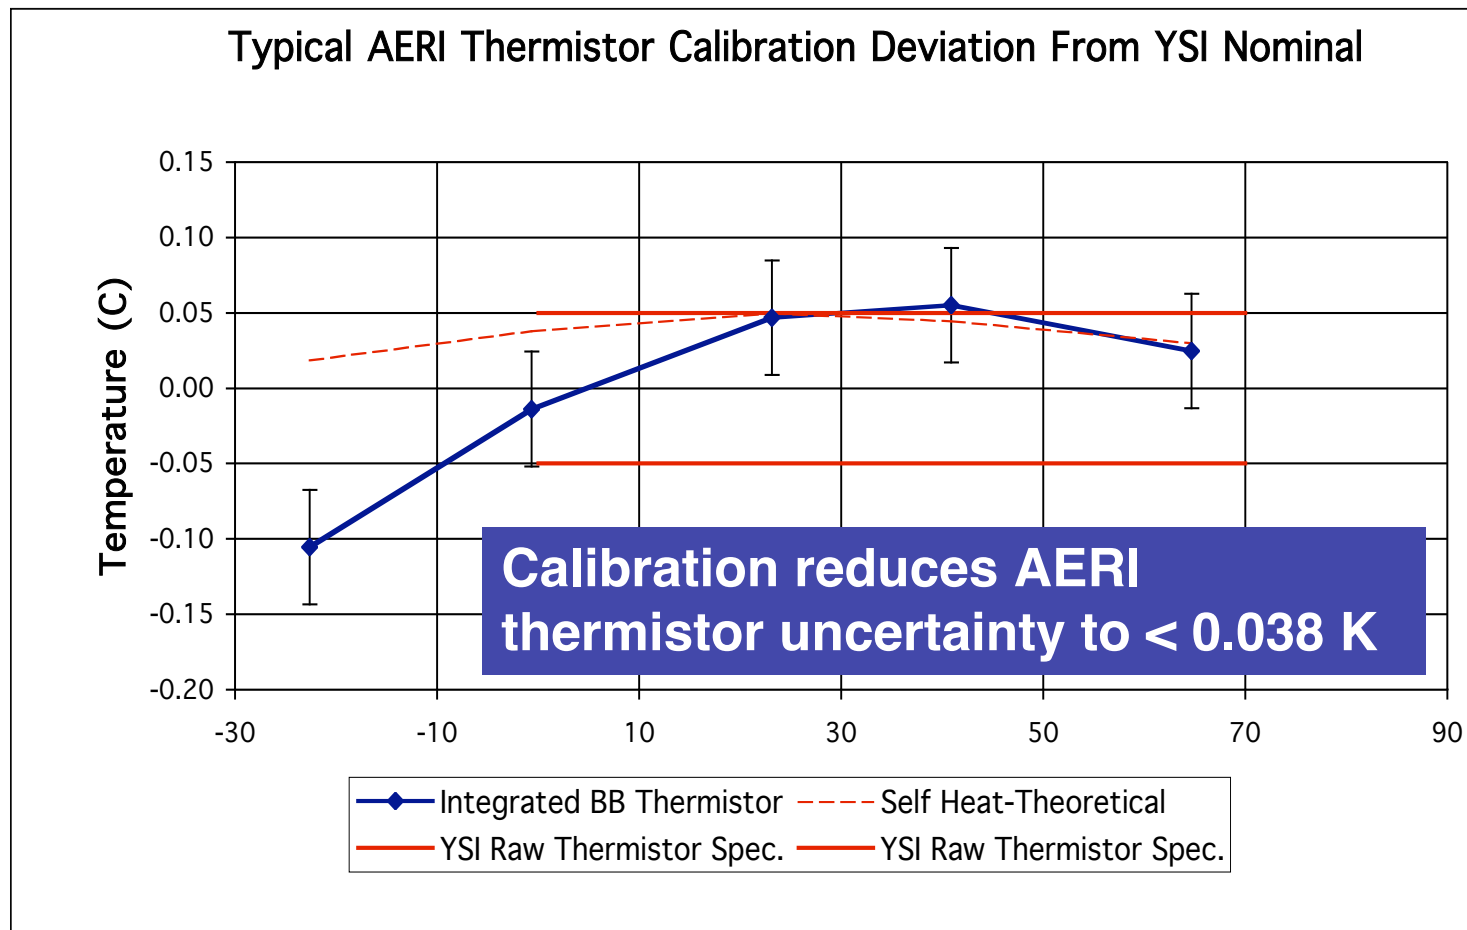

Data from AERI Blackbody S/N 34



Thermistor Calibration Residual Errors From Regression Fit of Steinhart and Hart Equations

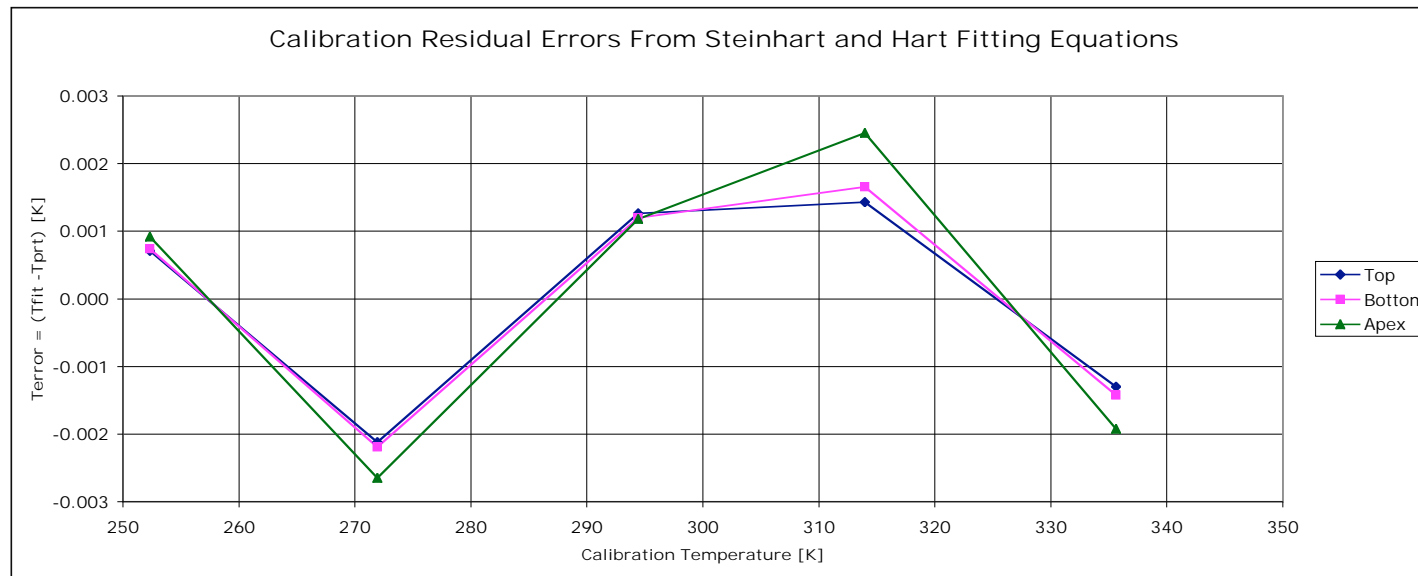

Residual Error From Fitting Equations < 3 mK


$$\frac{1}{T} = A + B \ln(R) + C(\ln(R))^3$$

Data from BB S/N 24



Temperature Gradient Due to Paint Thickness

Tamb = 20 C
Thbb = 60 C

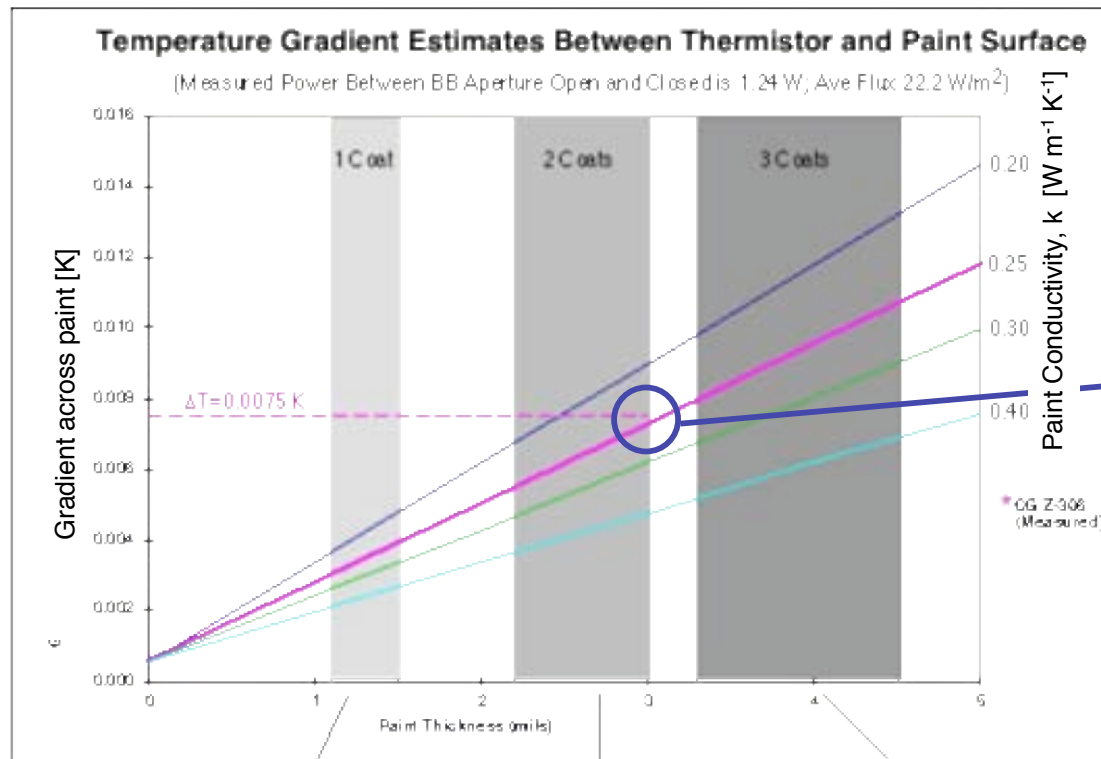


→ $\Delta T = 0.0075$ K
results from
(Th-Ta)=40 C.

→ ΔT expected to be
< 0.03 K
for max. expected
(Th-Ta)=120 C.

→ 0.03 K is carried in
the uncertainty
budget


$$\Delta T = (P/A) * (t/k)$$

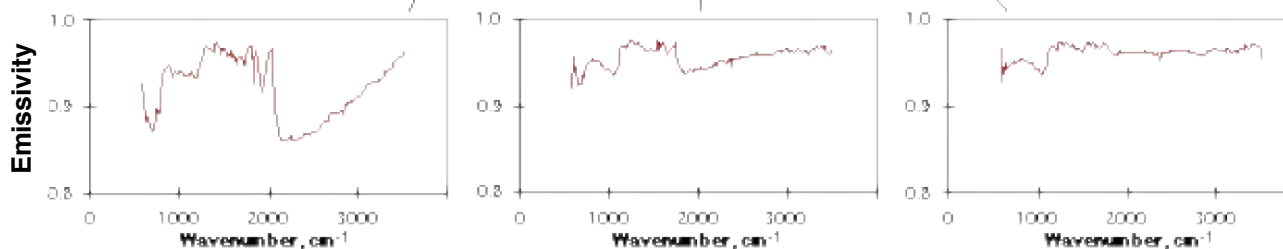


Typical Long-term Blackbody Thermistor Drift

**Long-term
Thermistor Drift
< 0.05 K**

**Data from AERI
Blackbody S/N 24**

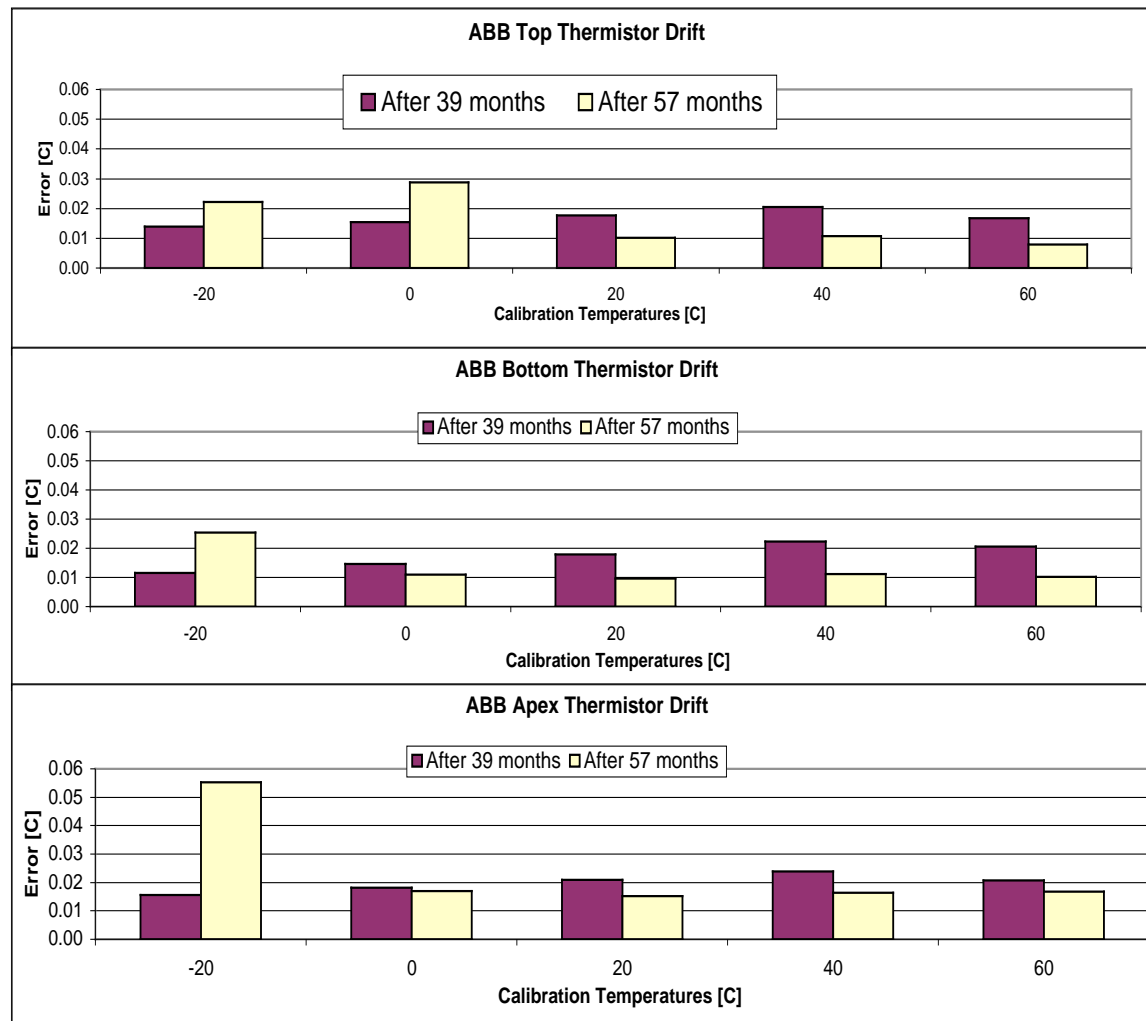


AERI Thermistor Resistance Measurement Electronics

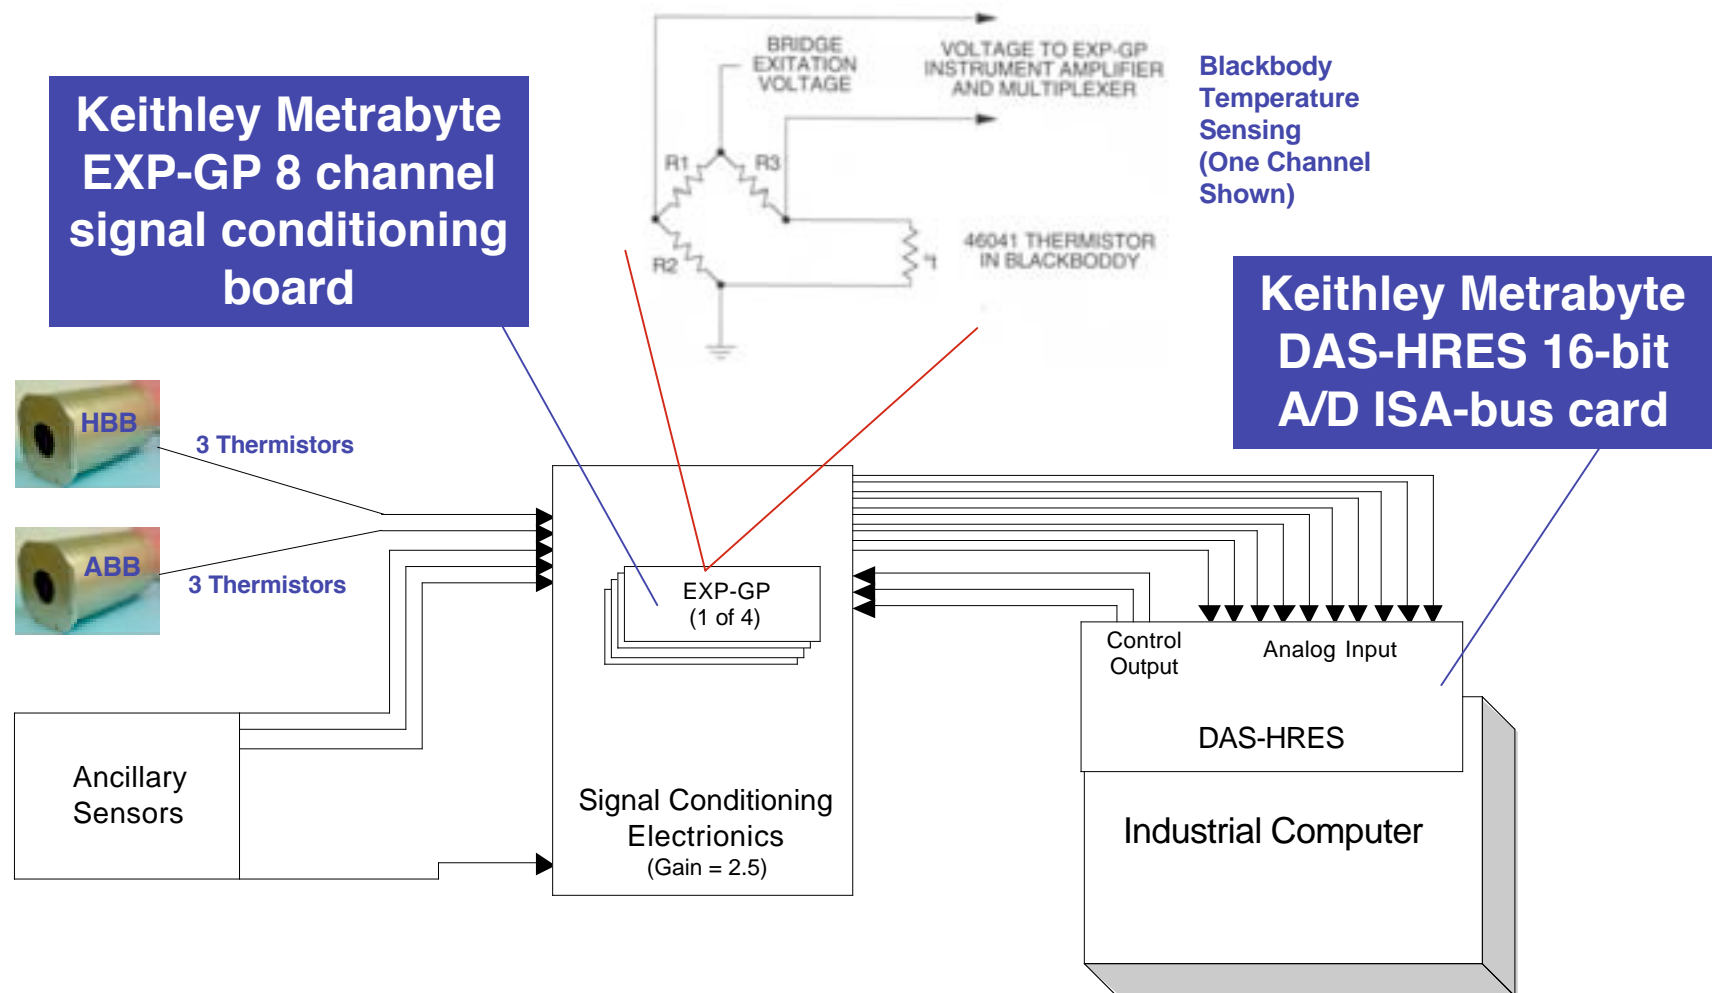

Calibration Resistor Traceability & Uncertainty

Uncertainty in Calibration Resistor Measurements Expressed as Equivalent Temperature Errors

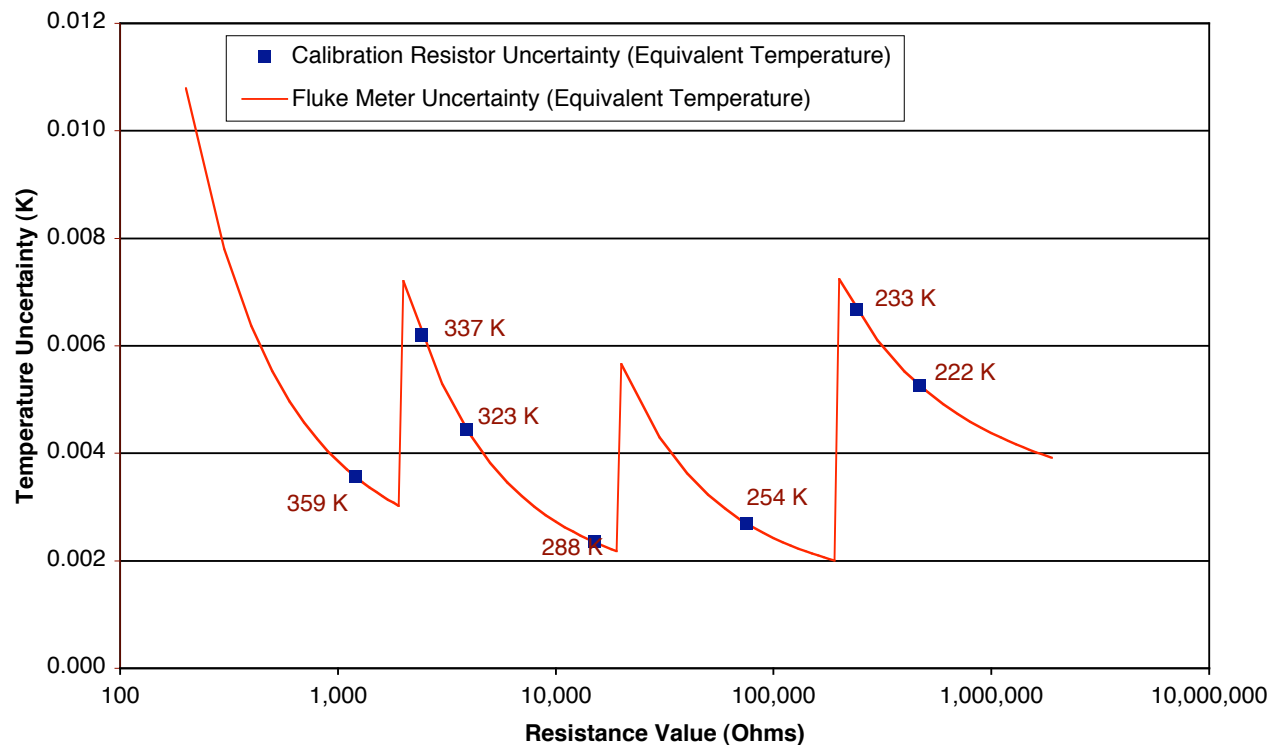


Calibration of AERI thermistor resistance measurement electronics uses precision resistors

Temperature error associated with calibration resistor uncertainty is $< 7 \text{ mK}$

UW SSEC 8842A Fluke Meter Calibrated at Factory using a Fluke 5700A-W/03 Calibrator Primary Standard Traceable to NIST



AERI Electronics Post Calibration Residuals

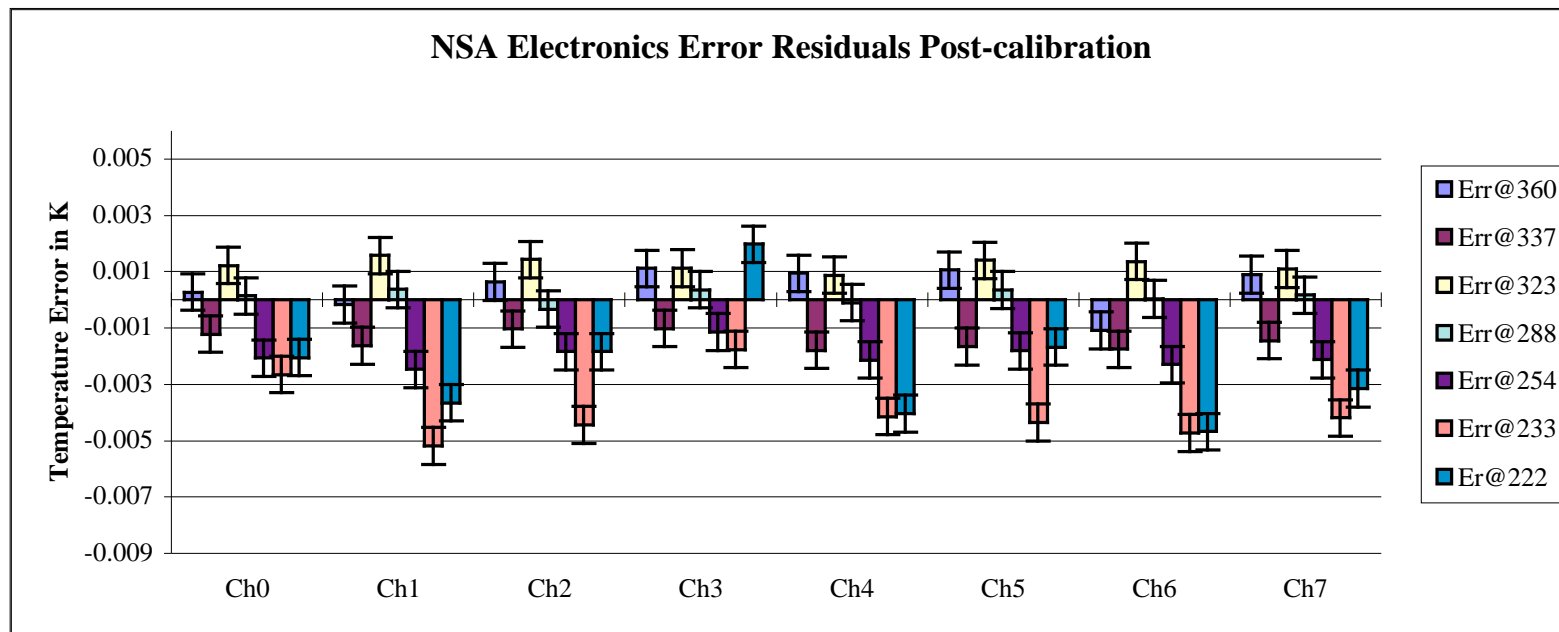


Equivalent temperature error following AERI electronics calibration is < 7 mK

**Residuals arise from linear fit in the Count Domain
Transformed to the Temperature Domain**




AERI Electronics Long-term Drift

Equivalent Temp of 336 K

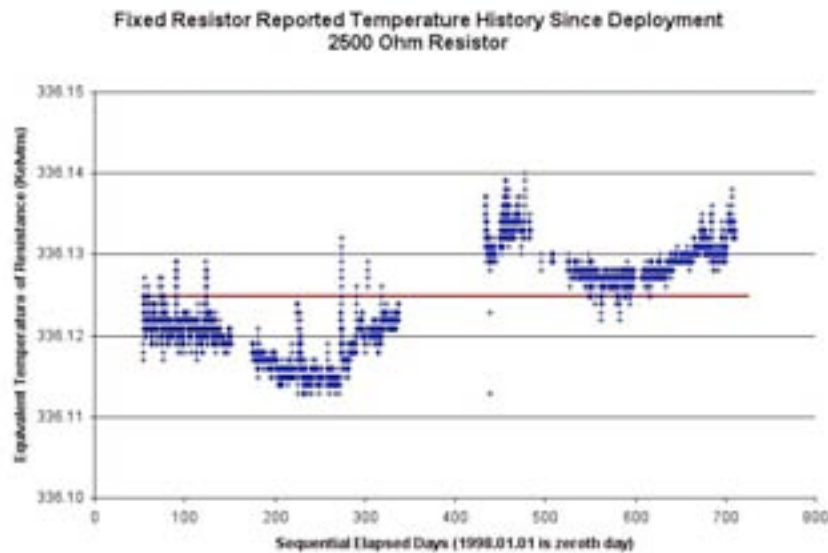

Equivalent Temp of 249 K

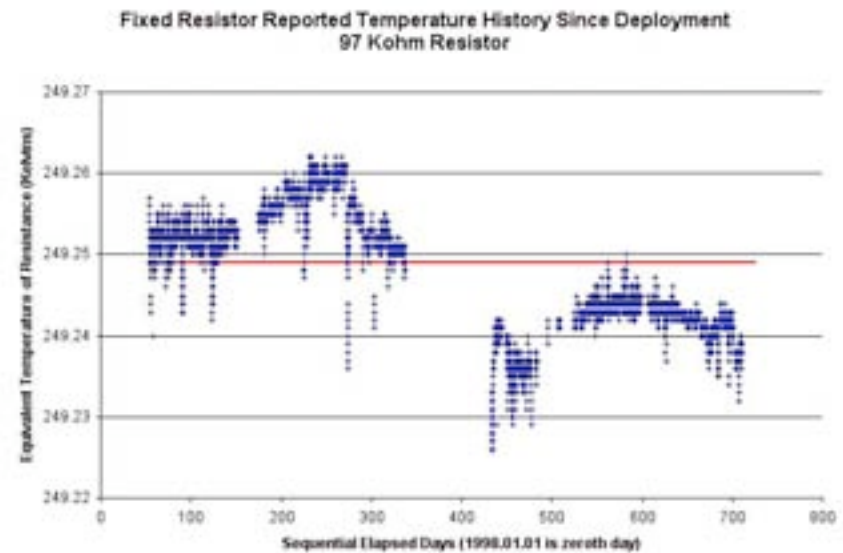

Temperature Error Associated With Long-term Drift of the Electronics is < 0.030 K



Emissivity Uncertainty Budget

		Uncertainty (3 sigma)	Note	for $E_p=0.94$ $f=39$	ΔE_c	ΔE_c (3 sigma)
36	Paint Witness Sample Measurement	1.5% E_p	[1]	$\Delta E_p=0.0141$	$(1/f)*\Delta E_p$	0.00036
36	Paint Application Variation	1.0% E_p	[2]	$\Delta E_p=0.0094$	$(1/f)*\Delta E_p$	0.00024
36	Long-term Paint Stability	2.0% E_p	[3]	$\Delta E_p=0.0188$	$(1/f)*\Delta E_p$	0.00048
39	Cavity Factor	30% f	[4]	$\Delta f=11.7$	$(1-E_p)/f^2*\Delta f$	0.00046
RSS						0.00080

Notes:

- [1] Factor of 4 higher than NIST* for 2 sigma. Another factor of 1.5 to get to 3 sigma.
- [2] Worst case difference between 1 and 3 coats
- [3] 2 x above
- [4] Accounts of Cavity Model Uncertainty

* NIST Stated accuracy is 4% of Reflectivity (2 sigma)

XX

Indicates slide number where more detailed information is presented

$$f=(1-E_p)/(1-E_c)$$

f =Cavity Factor

E_p =Emissivity of Paint

E_c =Emissivity of Cavity





Slide 35

CALCON 2003
Radiometric Calibration of AERI


THE UNIVERSITY
of
WISCONSIN
MADISON



Paint Emissivity Measurement

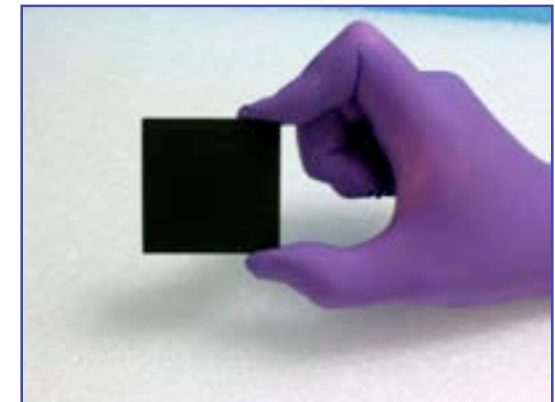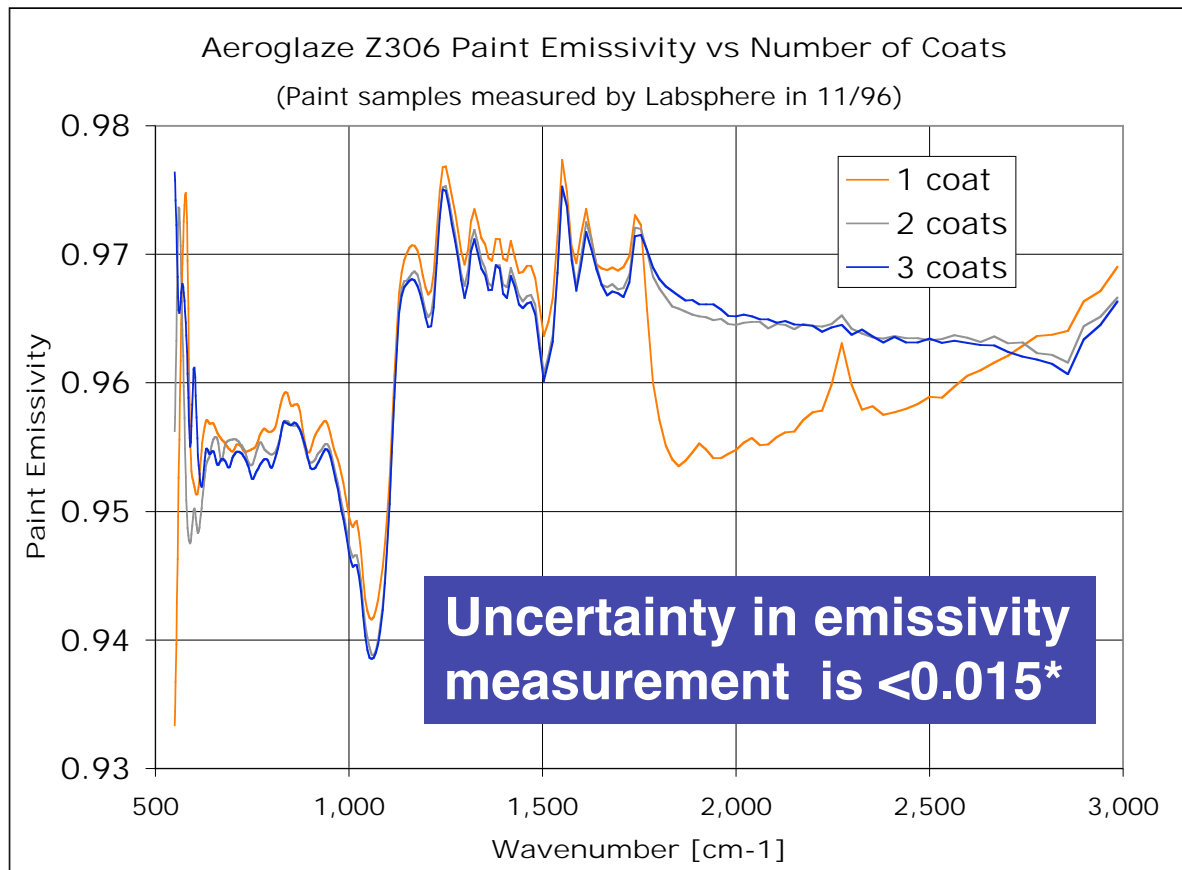

Blackbody Paint Witness Sample

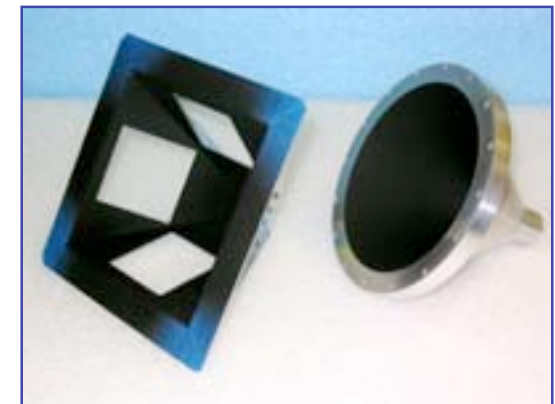

Witness Sample Holder "Mimics"
Blackbody Cone Geometry

**Labsphere does not state accuracy for high emissivity samples. Stated value is conservative. By comparison, NIST stated accuracy for this measurement is <0.004 .*




Emissivity Characterization From Monte Carlo Modeling

- Emissivity better than 0.998
- Emissivity knowledge: better than 0.001

$$R = \epsilon * B(T_{\text{eff}}) + (1 - \epsilon) * B(T_{\text{refl}})$$

$$T_{\text{eff}} = w_1 * T_A + w_2 * T_B$$

$B(T)$ = Planck radiance at T

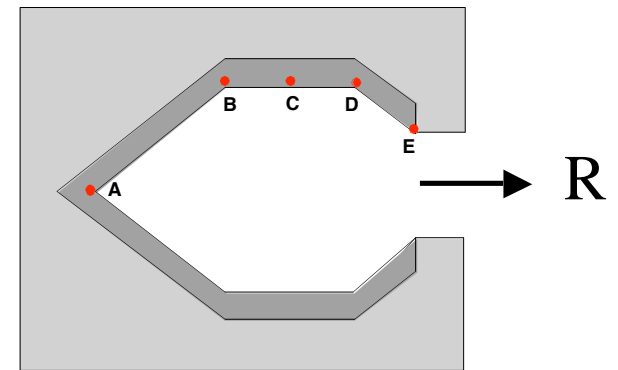



ϵ , w_1 , and w_2 are computed using a Monte Carlo based cavity model




Model of Thermal Gradients in Blackbody

$T_{amb} = 20\text{ C}$
 $T_{hbb} = 60\text{ C}$

Temperature
distribution
used in Monte
Carlo ray-
trace
determination
of T_{eff}

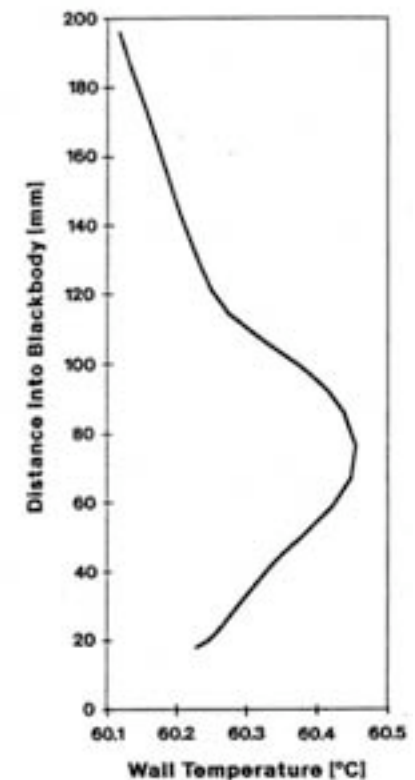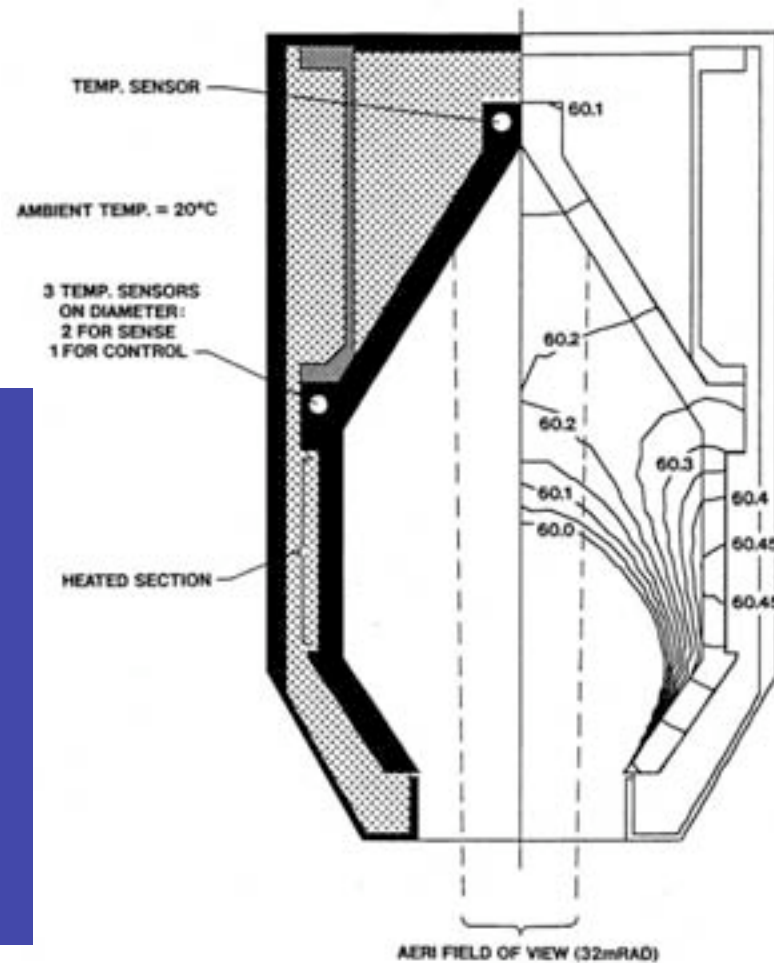



Monte Carlo Predictions of AERI Blackbody Cavity Emissivity (Diffuse Paint)

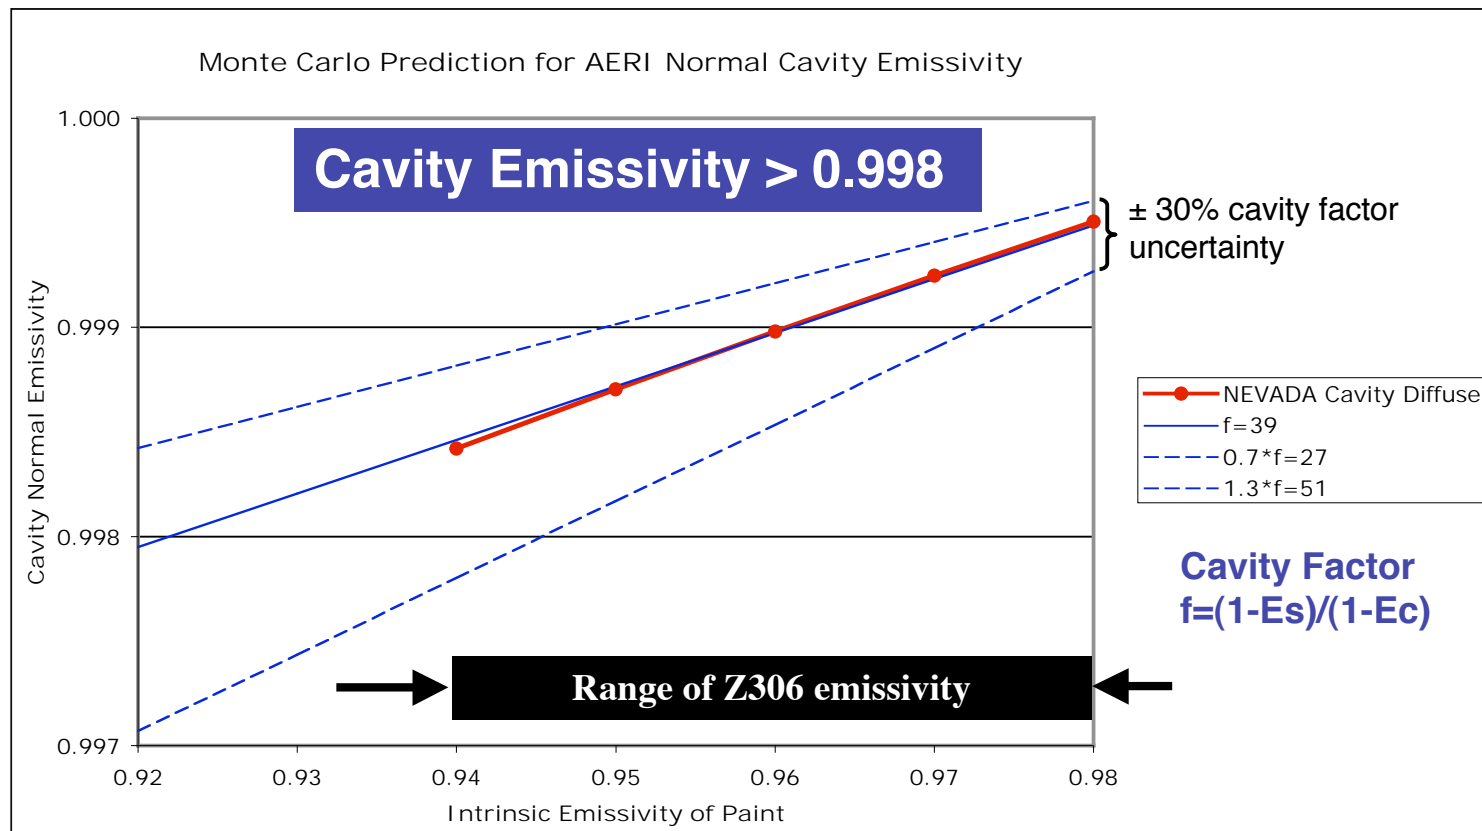

Deviations from the diffuse paint assumption equivalent to 20% specularity are within the cavity factor uncertainty of 30%.



AERI Radiometric FOV at Blackbody

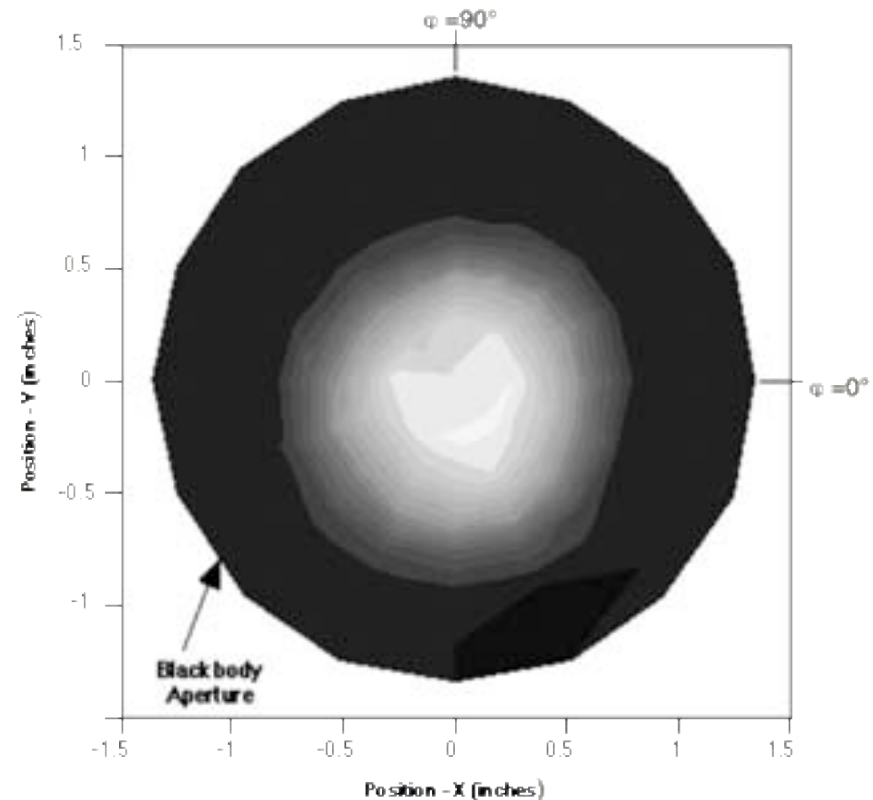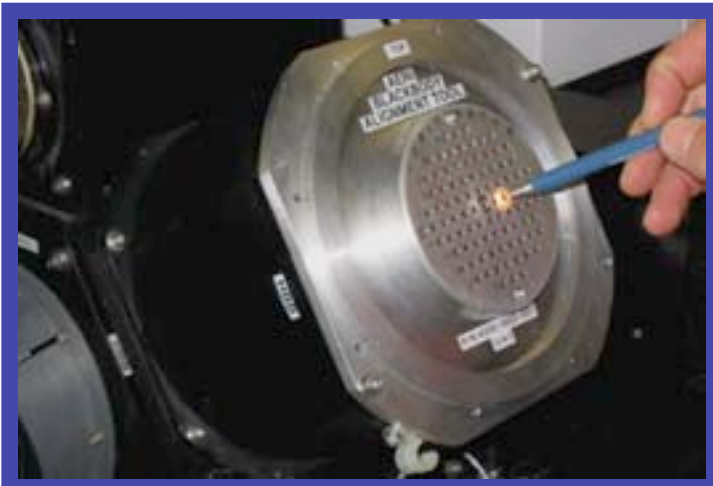

Radiometric Field-of-view is verified at the position of the blackbody aperture



Instrument End-to-end Performance



Slide 41


CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



AERI / NIST 3rd Generation Water-bath Based Blackbody Intercomparison - LW

Miami IR Workshop: 3-4 March 1998

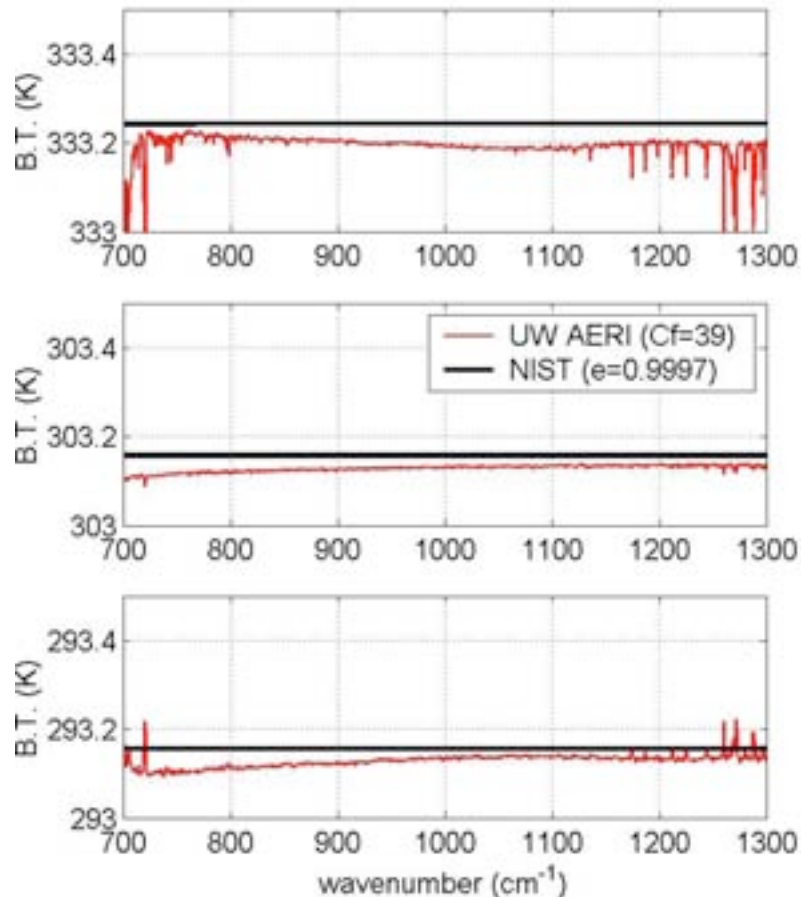


Max Error @ 333 K <0.055K
Max Error @ 303 K <0.050K
Max Error @ 293 K <0.050K



AERI / NIST 3rd Generation Water-bath Based Blackbody Intercomparison - SW

Miami IR Workshop: 3-4 March 1998

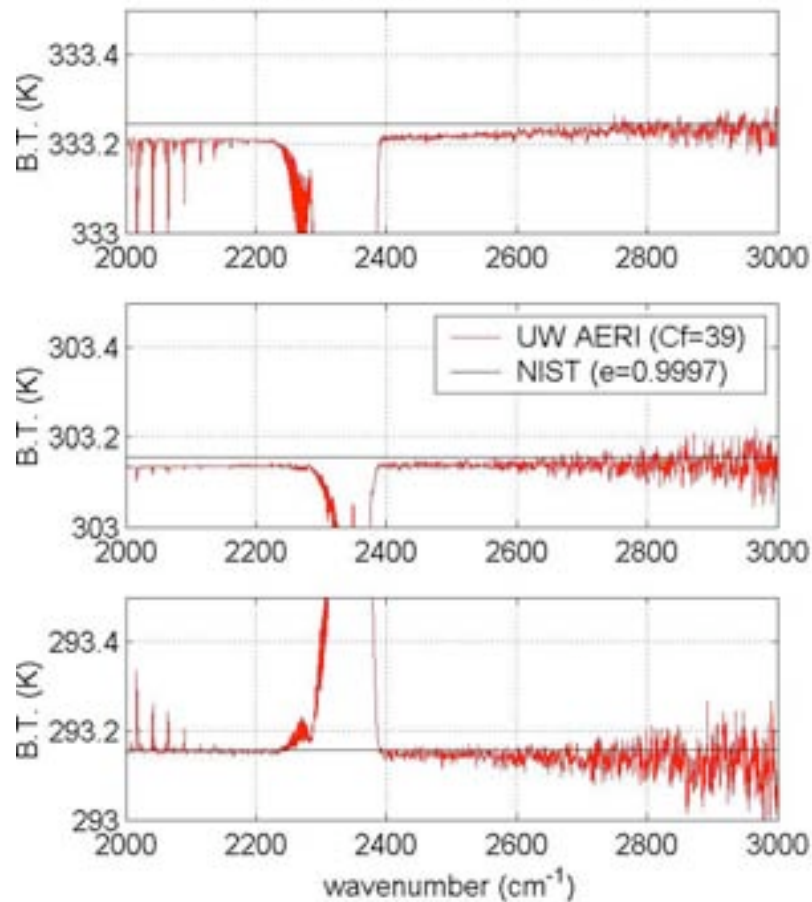

Max Error @ 333 K <0.035K
Max Error @ 303 K <0.025K
Max Error @ 293 K <0.035K




AERI Instrument End-to-end Radiometric Calibration Configuration




**AERI
Intermediate
Temperature
Blackbody in
Sky view**

**AERI Ice
Blackbody in
Down View**

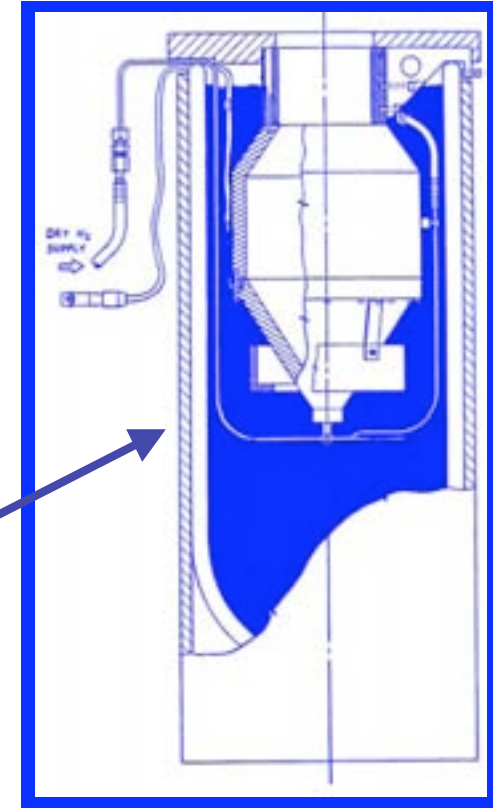


AERI Instrument End-to-end Radiometric Calibration

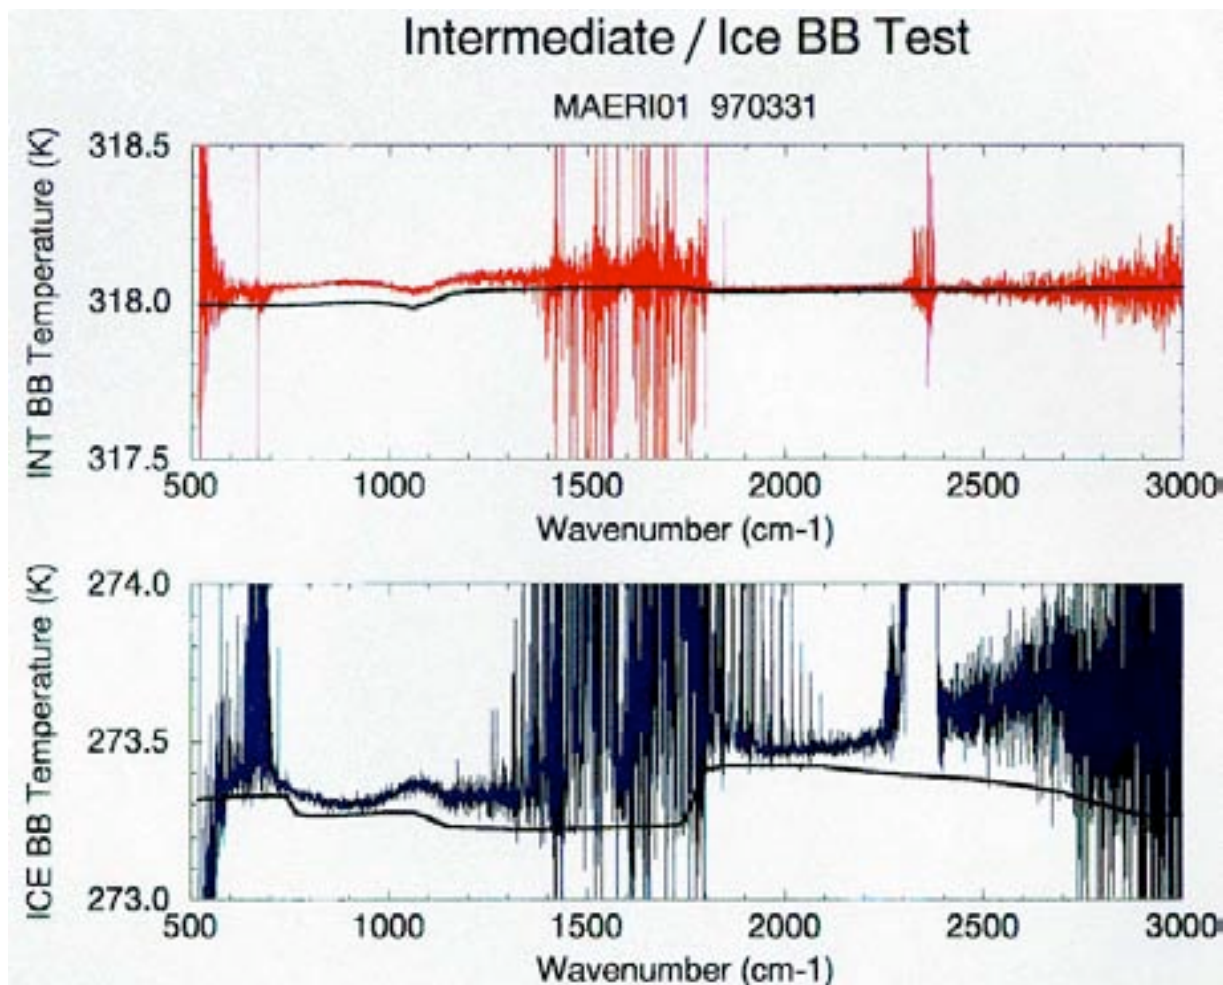

**General
Agreement
Better Than 0.1 K**



Calibration Variability Among 6 AERIs

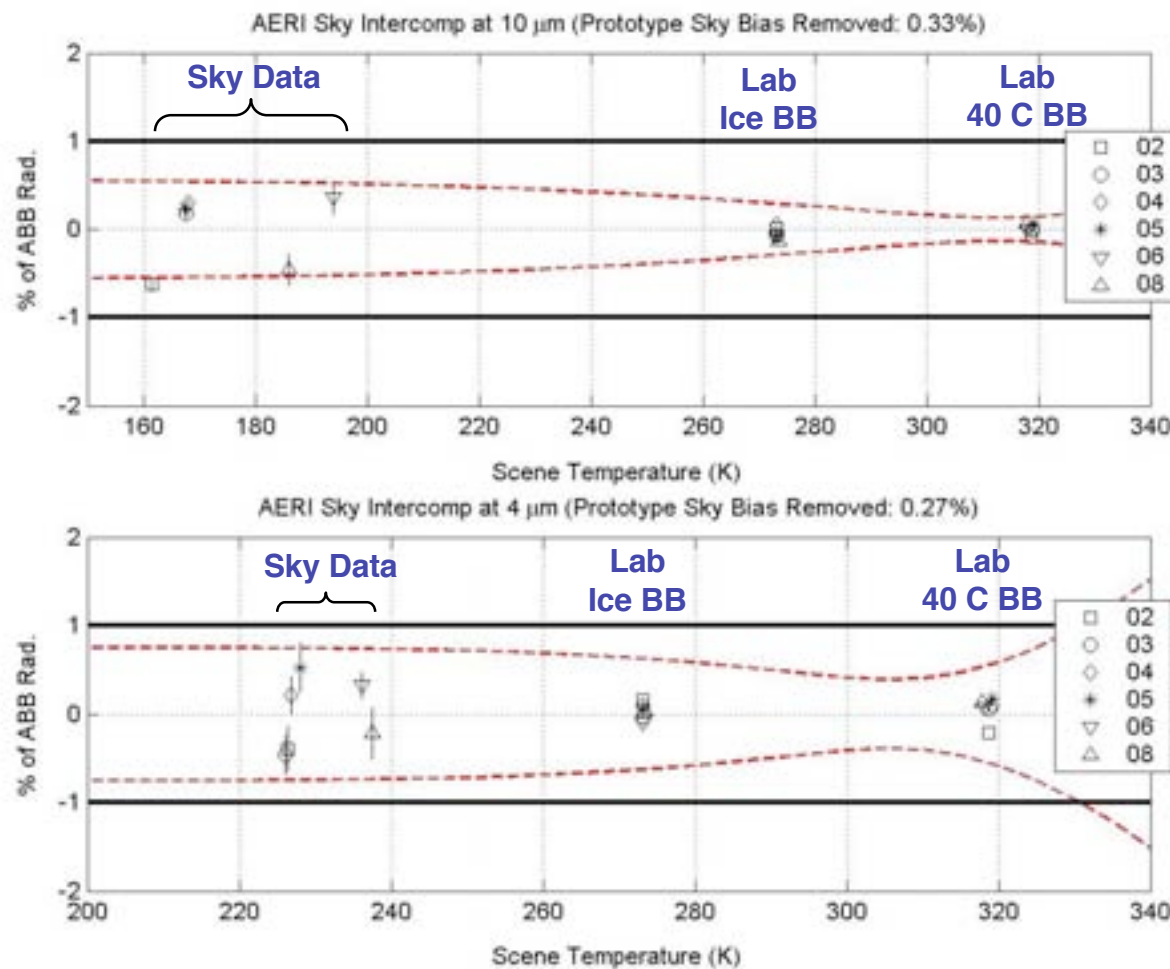


AERI Radiometric Model Accurately Predicts Performance

— 1% Specification
- - - Calibration Model




AERI Short Term Reproducibility


AERI-03 External BB Test (319K): UW-SSEC 12 Nov 1998

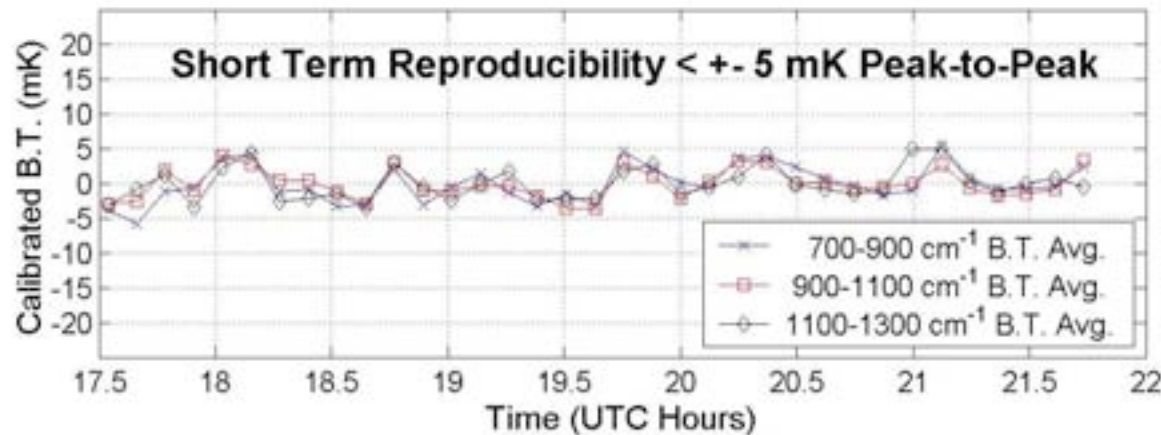

**AERI stability
better than 5 mK
over a period of
4 hours**

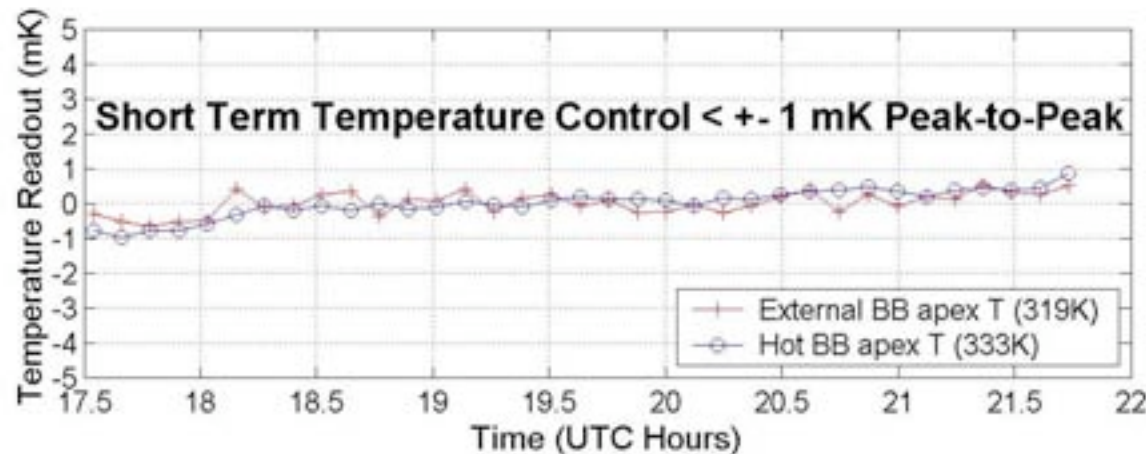


AERI Spectra Showing Reproducibility

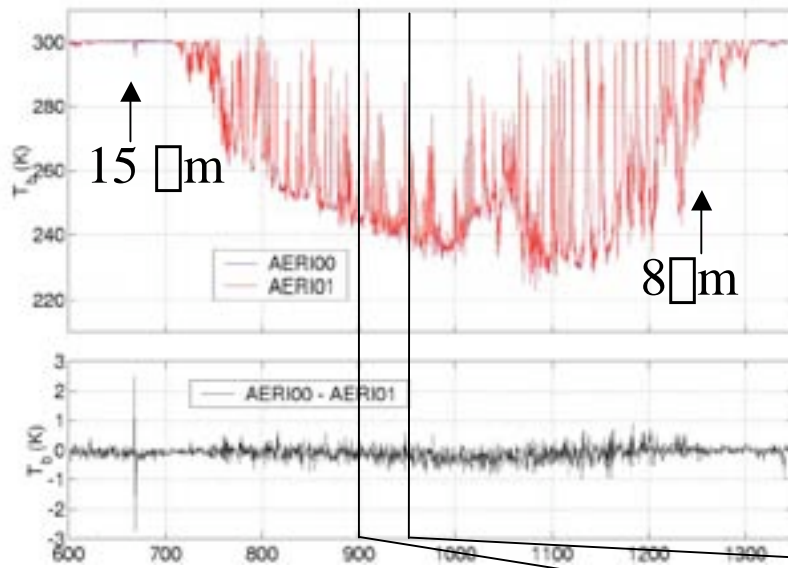


Wavenumbers (cm^{-1})

**Brightness
Temp Overlay of
2 Observations**

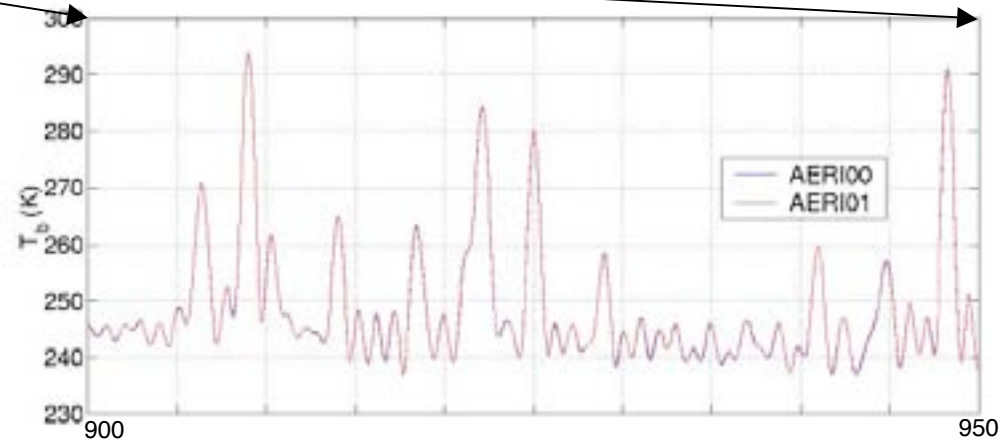


Intercomparison of Two MAERIs Measuring Sea Surface Temperature

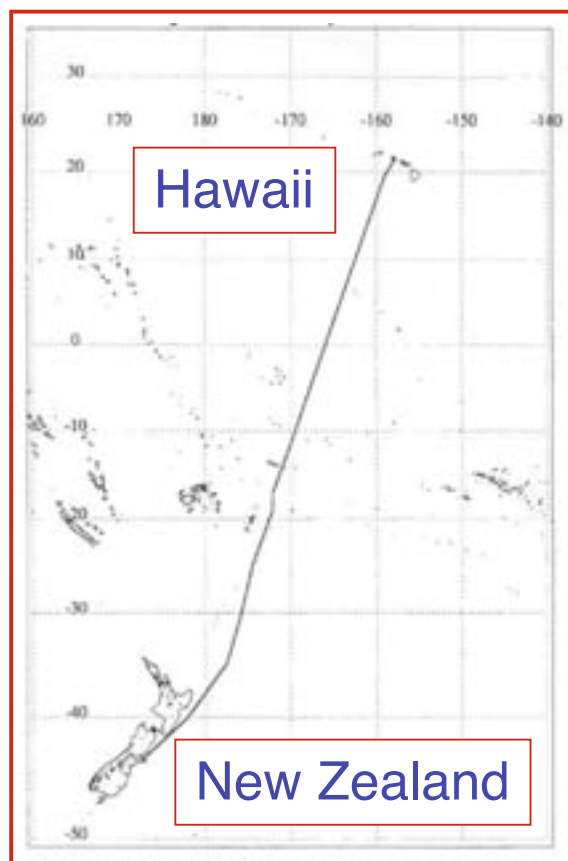

Track of the R/V Roger Revelle
28 Sept. - 14 Oct. 1997

16 Day Cruise

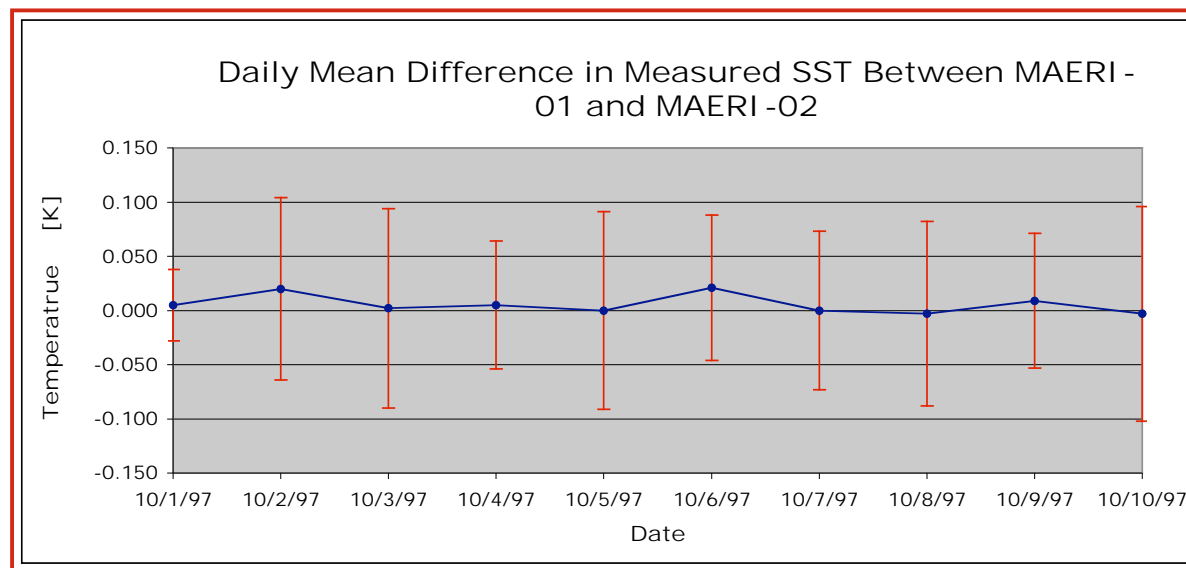

Largest Daily Mean Difference: 0.020 K
Ten Day Mean Difference: 0.005 K



Summary



Slide 50

CALCON 2003
Radiometric Calibration of AERI

THE UNIVERSITY
of
WISCONSIN
MADISON



Summary

- ❑ The AERI is a robust well calibrated spectroradiometer with a demonstrated absolute radiometric accuracy better than 1% of ambient radiance, making it an especially valuable tool for climate and remote sensing applications.
- ❑ **The AERI Calibration Blackbody performance and calibration methodology with Traceability to NIST have been verified.**
- ❑ Success of the AERI has led to the use of the same concept for aircraft instruments (S-HIS and NAST) and for the advanced geostationary sounder (GIFTS).
[see Dave Tobin and John Elwell, CALCON 2003]

